



MAXXAM ANALYTICS  
#1 2080 39 Ave. NE, Calgary, AB  
T2E 6P7

maxxam.ca  
Toll Free 800-386-7247  
Fax 403-219-3673

**AMBIENT AIR MONITORING MONTHLY DATA REPORT**  
**PEACE RIVER AREA MONITORING PROGRAM COMMITTEE**  
**THREE CREEKS 986B STATION**

**JOB #: 8449-2018-10-67-C**

**October 2018**

Prepared for:

**PEACE RIVER AREA MONITORING PROGRAM COMMITTEE**

**Attention: LILY LIN**

DATE: **November 19, 2018**

Prepared by:

A handwritten signature in blue ink, appearing to read "Wunmi Adekanmbi".

---

Wunmi Adekanmbi, M.Sc., EPt, PMP  
Project Team Lead, Customer Service, Air Services

Reviewed by:

A handwritten signature in black ink, appearing to read "Maram Ghaleb".

On behalf of:

---

Cheri Sinclair, B.Sc.  
Supervisor, Customer Service, Air Services

## **SUMMARY**

In October 2018, Maxxam Analytics was contracted to manage the ambient air quality monitoring and maintenance activities at the Three Creeks 986b Station, near Peace River Oil Sands Area 2, Alberta. The monitoring station provides continuous meteorological measurements and air quality data for non-compliance parameters, as requested by the PRAMP Committee.

All data collected this month was compliant with the requirements outlined in the Air Monitoring Directive (Alberta Environment and Parks, 2016).

The operational time for all continuous ambient air analyzers, meteorological systems and data acquisition systems were above the 90% requirement.

All data collected this month were within the Alberta Ambient Air Quality Objectives and Guidelines (November, 2018).

**SO<sub>2</sub>:** The analyzer was placed offline on October 10, at hour 18:00, for sample manifold cleaning, incurring one hour of downtime.

**THC/CH<sub>4</sub>/NMHC:** The analyzer was placed offline on October 1, at hour 09:00, while the fuel (H<sub>2</sub>) and carrier (N<sub>2</sub>) gas cylinders were being replaced. One hour of downtime was incurred.

The summary of results is presented on the following pages.

Any deviations or modifications made to the sampling or analytical methods are outlined in Section 1.0, Discussion. On this basis, Maxxam Analytics is issuing this completed report to Peace River Area Monitoring Program Committee.

Should you have any questions concerning the results or if we can be of further assistance, please contact us at 403-219-3661 or toll-free at 1-800-386-7247.

### Monthly Continuous Data Summary

Peace River Area Monitoring Program Committee						MAXIMUM VALUES							OPERATIONAL TIME (%)
Three Creeks 986b Station						1-HOUR					24-HOUR		
PARAMETER	OBJECTIVES		EXCEEDANCES		MONTHLY AVERAGE	READING	DAY	HOUR	WIND SPEED (kph)	WIND DIRECTION (sector)	READING	DAY	
	1-hr	24-hr	1-hr	24-hr									
SO <sub>2</sub> (ppb)	172	48	0	0	0	1	1	1	1.5	ESE	1	7	99.9
TRS (ppb)	-	-	-	-	0.31	2.25	15	22	1.7	SE	0.69	15	100.0
THC (ppm)	-	-	-	-	2.00	2.45	24	8	3.6	ESE	2.15	24	99.9
CH <sub>4</sub> (ppm)	-	-	-	-	2.00	2.44	24	8	3.6	ESE	2.15	24	99.9
NMHC (ppm)	-	-	-	-	0.00	0.01	15	10	2.1	WSW	0.00	1	99.9
RELATIVE HUMIDITY (%)	-	-	-	-	67	100	29	23	3.6	ESE	91	12	100.0
BAROMETRIC PRESSURE (millibar)	-	-	-	-	943	957	9	10	11.2	SE	955	9	100.0
AMBIENT TEMPERATURE (°C)	-	-	-	-	3.1	19.3	17	13	12.1	WSW	14.2	17	100.0
STATION TEMPERATURE (°C)	-	-	-	-	23.1	24.6	19	9	1.0	SSW	23.7	1	100.0
VECTOR WS (kph)	-	-	-	-	1.9	22.1	20	12	-	W	10.6	20	100.0
VECTOR WD (sec)	-	-	-	-	194 (SSW)	-	-	-	-	-	-	-	100.0

**SOUR GAS PROCESSING INDUSTRY  
MONTHLY REPORT SUMMARY**

**Three Creeks 986b Station**

**Peace River Area Monitoring Program Committee**

Plant Name / Location

Company

Licence Number	Report Date	
	YEAR	MONTH
N/A	2018	October

CONTINUOUS AMBIENT MONITORING						
PARAMETER	% TIME OPERATIONAL	ONE - HOUR AVERAGE			24 - HOUR AVERAGE	
		MAXIMUM VALUES	NO. READINGS > REGULATION	MAXIMUM VALUES	NO. READINGS > REGULATION	
SO <sub>2</sub>	99.9	0.001 ppm	0	0.001 ppm	0	
TRS	100.0	0.002 ppm	-	0.001 ppm	-	
THC	99.9	2.45 ppm	-	2.15 ppm	-	
CH <sub>4</sub>	99.9	2.44 ppm	-	2.15 ppm	-	
NMHC	99.9	0.01 ppm	-	0.00 ppm	-	
RH	100.0	100 %	-	91 %	-	
BP	100.0	957 mb	-	955 mb	-	
Ambient TPX	100.0	19.3 °C	-	14.2 °C	-	
Station TPX	100.0	24.6 °C	-	23.7 °C	-	
Wind Speed	100.0	22.1 kph	-	10.6 kph	-	
Wind Direction	100.0	-	-	-	-	

SIGNATURE OF COMPANY REPRESENTATIVE

FOR ALBERTA ENVIRONMENT USE ONLY

---

## Exceedance Summary Report

---

### SO<sub>2</sub> 1-Hour Exceedances

Measured concentrations of sulphur dioxide were below the 1-hour AAAQO of 172 ppb.

### SO<sub>2</sub> 24-Hour Exceedances

Measured concentrations of sulphur dioxide were below the 24-hour AAAQO of 48.0 ppb.

*In accordance with EPEA and the Substance Release Regulation.*

*In accordance with A Guide to Release Reporting and the Alberta Ambient Air Quality Objectives and Guidelines Summary.*

**TABLE OF CONTENTS**

<u>Title</u>	<u>Page</u>
<b>SUMMARY</b>	<b>2</b>
<b>MONTHLY CONTINUOUS DATA SUMMARY REPORT</b>	<b>3</b>
<b>SOUR GAS SUMMARY REPORT</b>	<b>4</b>
<b>EXCEEDANCE SUMMARY REPORT</b>	<b>5</b>
<b>TABLE OF CONTENTS</b>	<b>6</b>
<hr/>	
<b>1.0 Discussion</b>	<b>8</b>
<hr/>	
<b>2.0 Project Personnel</b>	<b>10</b>
<hr/>	
<b>3.0 Plant Monthly Required AMD Summary</b>	<b>10</b>
<hr/>	
<b>4.0 Calculations and Results</b>	<b>10</b>
<hr/>	
<b>5.0 Methods and Procedures</b>	<b>11</b>
<hr/>	
<b>Appendix I</b>	<b>Continuous Monitoring Data Results 14</b>
	<b>Sulphur Dioxide 15</b>
	<b>Total Reduced Sulphur 21</b>
	<b>Total Hydrocarbon 27</b>
	<b>Methane 33</b>
	<b>Non-Methane Hydrocarbon 39</b>
	<b>Wind Speed 45</b>
	<b>Wind Direction 50</b>
	<b>Relative Humidity 54</b>
	<b>Barometric Pressure 57</b>
	<b>Ambient Temperature 60</b>
	<b>Station Temperature 63</b>
<b>Appendix II</b>	<b>Equipment Calibration Results 66</b>
	<b>Sulphur Dioxide 67</b>
	<b>Total Reduced Sulphur 70</b>
	<b>Total Hydrocarbon 73</b>
	<b>Wind System 77</b>
	<b>Meteorological System Check 79</b>

	<b>Calibrators</b>	<b>81</b>
	<b>Calibration Gases</b>	<b>84</b>
<b>Appendix III</b>	<b>Maximum Instantaneous Data</b>	<b>88</b>
<b>Appendix IV</b>	<b>Report Certification Form</b>	<b>101</b>
<b>Appendix V</b>	<b>Data Validation Certification Form</b>	<b>103</b>

## **1.0 Discussion**

This monthly report consists of continuous monitoring results for the following parameters: Sulphur Dioxide (SO<sub>2</sub>), Total Reduced Sulphur (TRS), Total Hydrocarbon (THC), Methane (CH<sub>4</sub>), Non-Methane Hydrocarbon (NMHC), Relative Humidity (RH), Barometric Pressure (BP), Ambient Temperature (AmbTPX), Station Temperature (StnTPX), Wind Speed (WS) and Wind Direction (WD).

The sample inlet filter for all continuous air analyzers are replaced before the calibration begins. The sample manifold is cleaned during the site visit each month.

Control checks, consisting of a zero and span, are conducted daily on all continuous air monitors. In place of the air sample, zero air (from scrubbed air or gas cylinders) is used for zero checks, and a known concentration of the pollutant being analyzed is used for span checks. These checks are controlled by automatic timers and valves. The total zero span cycle is completed within an hour, the commencement of the zero span cycle is at the beginning of the hour.

Multipoint calibrations are done a minimum of once a month for each continuous air monitor. An additional calibration is required under the following conditions: 1) within three days after the initial start-up and stabilization of a newly installed instrument, 2) prior to shut-down or moving of an instrument which has been working to specification, and 3) when major repair has been done on the instrument.

Time during the first multi-point calibration is not considered downtime (Data is flagged as C). If more than one calibration is performed during the month, the time during the additional calibration is considered as downtime (Data is flagged as C1).

Only one zero/span check is run per day. Time during the zero/span check is not considered as downtime (Data is flagged as S). If an extra zero/span check is performed, the time during the additional check is considered as downtime (Data is flagged as S1).

The AMD requires each instrument and accompanying data recording system to be operational 90% of the time, at a minimum, for each monthly monitoring period.

All sampling, analysis, and QA/QC for this project was performed by Maxxam Analytics and complies with the Alberta Air Monitoring Directive.

Data contained in this monthly report has undergone verification and validation based on the requirements of the AMD (December, 2016) Chapter 6: Ambient Data Quality and Chapter 9: Reporting. The descriptions of the data verification and validation process can be found in Section 5 of this report. Instantaneous data, where applicable, is provided for reference purposes and has not undergone zero correction. The minimum and maximum statistics are highlighted in the data table and are for reference only. The highlighted cells are based on the software's interpretation of the exact position of the minimum or maximum value. The visual presentation of these statistics may not be the obvious choice in a data range due to rounding, truncating or analyzer specifications.

Hourly/minute data have been reviewed based on daily zero/span results and multi-point calibration results. Data may be considered invalid if a zero-corrected span check in excess of +/- 10% of the span concentration (established by the previous multi-point calibration) is encountered and/or significant differences in the calibration factor occurs (greater than 10%).



#### **SULPHUR DIOXIDE (SO<sub>2</sub>)**

- Operational time for the monitoring period was 99.9%, equivalent to one hour of downtime. This was incurred on October 10 at hour 18:00, as the analyzer was placed offline for sample manifold cleaning.
- The routine monthly calibration was performed on October 11.

#### **TOTAL REDUCED SULPHUR (TRS)**

- Operational time for the monitoring period was 100%.
- The routine monthly calibration was performed on October 10.

#### **TOTAL HYDROCARBONS (THC), METHANE (CH<sub>4</sub>) and NON-METHANE HYDROCARBONS (NMHC)**

- Operational time for the monitoring period was 99.9%, equivalent to one hour of downtime. This was incurred on October 1 at hour 09:00, as the analyzer was placed offline while the fuel (H<sub>2</sub>) and carrier (N<sub>2</sub>) gas cylinders were being replaced.
- The routine monthly calibration was performed on October 10.
- The canister sampler is programmed to draw in a whole air sample when the 5-minute average concentration of NMHC is above 0.30 ppm. A representative sample of ambient air is collected over a one-hour period when the canister event is triggered. No canister event was recorded this month. A trigger test was performed during the routine monthly calibration on October 10 to assess the effectiveness of the canister system. No deficiencies were found.

#### **WIND SPEED (WS) and WIND DIRECTION (WD)**

- Operational time for the monitoring period was 100%.
- An anemometer sensor check was conducted on October 10. The result was satisfactory.
- Wind data is reported as vector wind speed and vector wind direction. Wind direction is defined as the direction from which the wind is blowing from and is measured in degrees from true north.

#### **RELATIVE HUMIDITY (RH)**

- Operational time for the monitoring period was 100%.
- A humidity sensor check was conducted on October 10. The result was satisfactory.

#### **BAROMETRIC PRESSURE (BP)**

- Operational time for the monitoring period was 100%.
- A pressure sensor check was conducted on October 10. The result was satisfactory.

#### **AMBIENT TEMPERATURE (AmbTPX)**

- Operational time for the monitoring period was 100%.
- A temperature sensor check was conducted on October 10. The result was satisfactory.

#### **STATION TEMPERATURE (StnTPX)**

- Operational time for the monitoring period was 100%.

---

## **2.0 Project Personnel**

Karla Reesor was the contact for Peace River Area Monitoring Program Committee and the Maxxam field technician was Limin Li.

## **3.0 Plant Monthly Required AMD Summary**

All data collected this month was compliant with the requirements outlined in the Air Monitoring Directive (Alberta Environment and Parks, 2016).

The operational time for all continuous ambient air analyzers, meteorological systems and data acquisition systems were above the 90% requirement.

All data collected this month were within the Alberta Ambient Air Quality Objectives and Guidelines (November, 2018).

## **4.0 Calculations and Results**

All calculations and reporting of results follow the methods described in the AMD, 2016.

## 5.0 Methods and Procedures

The following methods and procedures were used to complete the monitoring program:

Maxxam AIR SOP-00001: Methane, Non-Methane Hydrocarbon Analyzer Monitoring

Maxxam AIR SOP-00013: RM Young Wind Monitor Calibration

Maxxam AIR SOP-00209: Ambient Sulphur Monitoring

There were no deviations from the prescribed methods.

The following instruments were used to perform the test program:

Sulphur Dioxide - Thermo 43C UV Fluorescent Analyzer

Total Reduced Sulphur - Thermo 43i - TLE UV Fluorescent Analyzer

Methane, Non-Methane Hydrocarbon - Thermo 55i FID Analyzer

Wind System - RM Young Unit

Relative Humidity - RM Young Unit

Barometric Pressure - Met One Unit

Ambient Temperature - RM Young Unit

Datalogger - Envidas Ultimate

The following steps were used to complete the data verification and validation process:

**Level 0 Preliminary Verification**

Level 0 data are raw data obtained directly from the data acquisition system (DAS). Under the step of Level 0, these data undergo a certain amount of manual or automated screening and flagging. It included a) identification of periods of missing data; b) verification of time stamps against reference time; c) verification that instrument diagnostics/datalogger flags indicate normal operation; d) comparison of data to upper and lower limits; e) rate of change flagging indicating that data changed too rapidly or not at all; and f) verification that zero, span and multipoint performance checks are within specifications. This level of verification is performed on a daily basis.

**Level 1 Primary Validation**

Validation actions under the step of Level 1 include a) review of all screening flags assigned during preliminary verification; b) review of all supporting site information and documentation; c) review of operational acceptance limits for each parameter/analyzer; d) review of daily zero/span and monthly calibration results for all gaseous parameters; and e) application of any necessary adjustments to data (e.g. baseline adjustments, below zero adjustments). This level of validation is performed on a monthly basis.

**Level 2 Final Validation**


The purpose of Level 2 validation is to verify that there are no inconsistencies among related data, or among regional data measured at nearby sites.

**Level 3 Independent Data Review**

Level 3 validation is the last step of data review, and it is completed by an individual that is independent of both field operations and primary data validation. A final independent QA review and endorsement is performed during this step before data is submitted to Alberta Environment.

**Post-Final Validation**

The Post-Final Validation step serves to re-evaluate the data that errors or omissions are discovered and/or suspected after the initial submittal of data. Any data issues or patterns which were not clear on a monthly basis are highlighted during this step. This validation is performed on an annual basis.

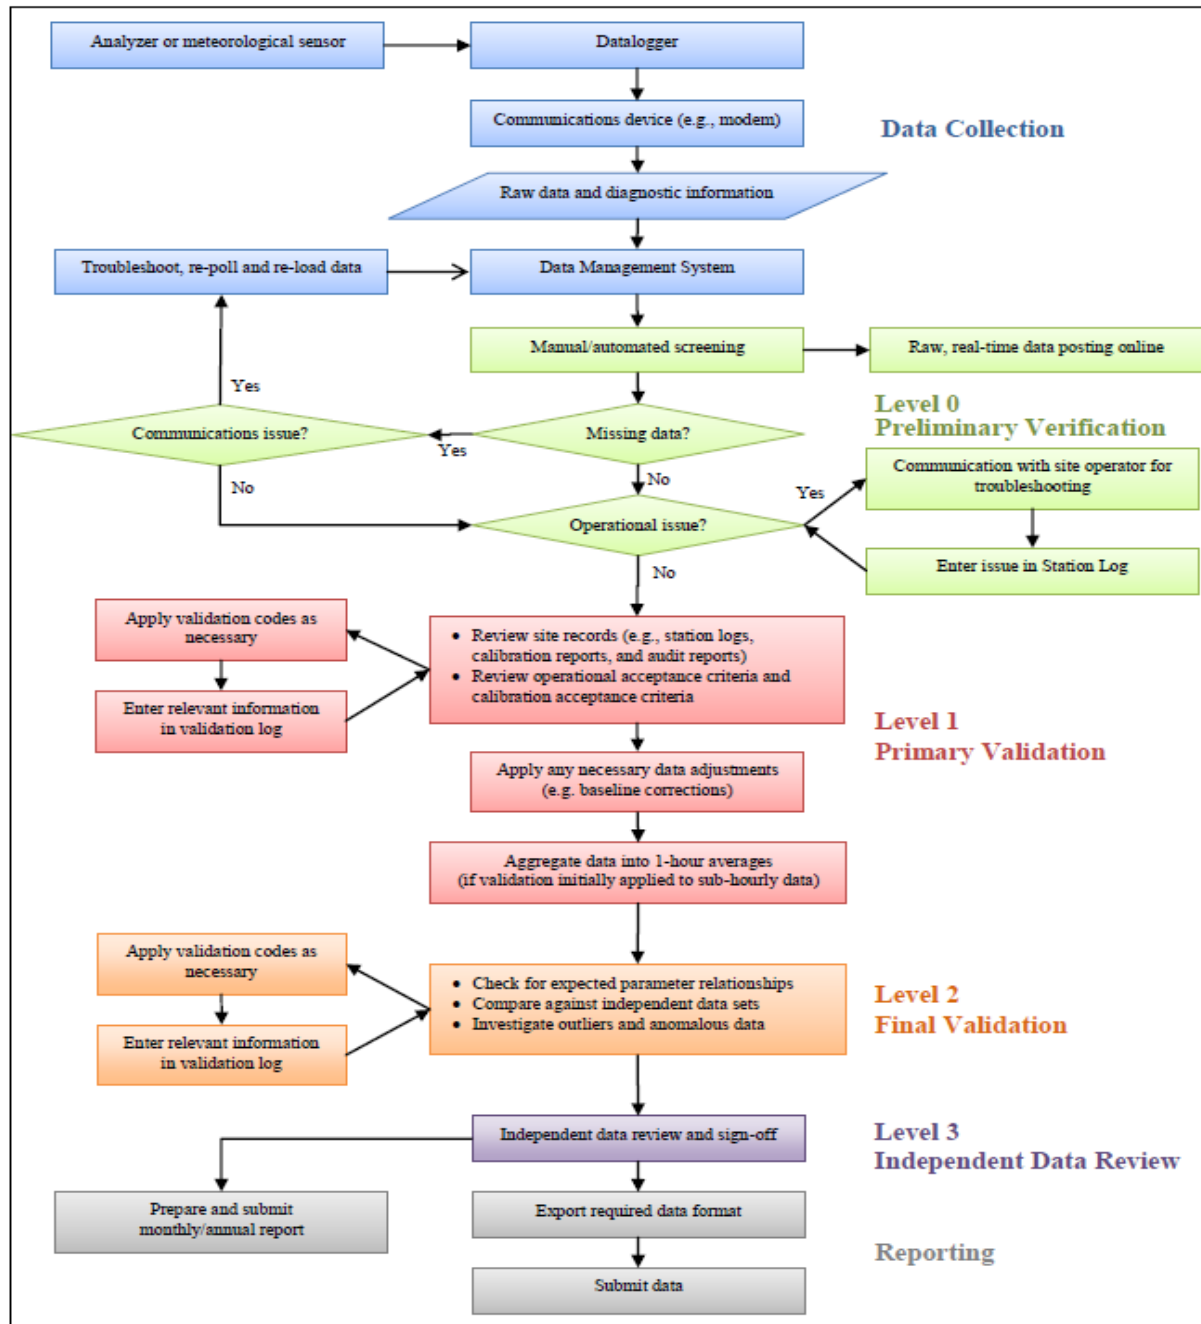

Source: Air Monitoring Directive (December 2016), Chapter 6, Ambient Data Quality; Figure 1 Data Collection and Management Process Flow Chart

***APPENDIX I***  
***CONTINUOUS MONITORING DATA RESULTS***

***SULPHUR DIOXIDE***

SULPHUR DIOXIDE Hourly Averages (SO<sub>2</sub> ppb)

HR START (MST)	0:00	1:00	2:00	3:00	4:00	5:00	6:00	7:00	8:00	9:00	10:00	11:00	12:00	13:00	14:00	15:00	16:00	17:00	18:00	19:00	20:00	21:00	22:00	23:00	DAILY	DAILY	24-HR	RDGS.	
HR END (MST)	0:59	1:59	2:59	3:59	4:59	5:59	6:59	7:59	8:59	9:59	10:59	11:59	12:59	13:59	14:59	15:59	16:59	17:59	18:59	19:59	20:59	21:59	22:59	23:59	MIN.	MAX.	AVG.		
DAY																													
1	0	1	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	S	0	0	0	1	1	0	24
2	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	24
3	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	0	0	24
4	1	0	0	0	0	1	1	0	0	0	0	0	0	1	0	0	1	1	S	0	0	0	0	0	0	0	1	0	24
5	0	0	0	0	0	0	0	0	0	0	1	0	1	0	1	1	1	S	1	0	1	1	1	1	1	0	1	0	24
6	1	0	0	0	0	1	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	0	0	0	0	1	0	24
7	0	0	0	0	1	1	0	0	0	1	0	1	1	1	S	1	0	0	0	0	1	1	1	1	0	1	1	0	24
8	1	0	0	0	0	1	0	1	1	1	1	1	1	S	1	1	1	0	0	0	0	0	0	0	0	1	0	0	24
9	0	0	0	0	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	0	0	0	0	0	0	0	0	24
10	0	0	0	0	0	0	0	0	0	1	0	0	S	0	0	0	0	0	Y	0	0	0	0	0	0	0	1	0	23
11	0	0	0	0	0	0	0	C	C	C	0	S	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	24
12	0	0	0	0	0	0	1	1	0	1	S	0	1	1	0	0	0	0	0	0	0	0	0	0	1	0	1	0	24
13	0	0	0	0	0	0	0	0	0	S	0	0	0	0	1	0	0	0	0	0	0	0	0	0	0	0	1	0	24
14	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	1	0	0	1	0	0	1	0	0	0	1	0	24
15	0	1	1	1	1	1	1	S	1	1	1	1	1	0	0	0	0	0	0	0	0	0	0	0	0	0	1	0	24
16	0	0	0	0	0	0	S	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	24
17	0	0	0	0	0	S	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	24
18	1	1	1	0	S	1	1	1	1	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	1	0	24
19	0	0	0	S	0	0	0	0	0	0	1	1	1	0	0	0	0	0	0	0	0	0	0	0	0	0	1	0	24
20	0	0	S	0	0	0	0	0	0	0	0	0	0	1	0	1	0	0	0	0	0	0	0	0	0	0	1	0	24
21	0	S	0	0	0	0	1	0	1	1	1	1	0	0	1	0	1	0	0	0	0	0	0	0	0	0	1	0	24
22	S	0	0	0	0	0	0	0	0	1	1	1	1	0	0	0	0	0	0	0	0	0	0	0	S	0	1	0	24
23	0	0	0	0	1	0	0	0	0	0	0	1	1	0	0	1	0	0	0	0	0	0	0	S	0	0	1	0	24
24	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	24
25	0	0	0	0	0	0	0	0	0	0	0	1	1	1	1	0	0	1	1	S	1	1	1	1	0	1	0	0	24
26	1	1	0	0	0	0	0	0	0	0	0	0	0	0	1	0	0	0	0	S	0	0	0	0	0	0	1	0	24
27	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	0	0	0	24
28	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	0	0	0	24
29	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	0	0	0	0	24
30	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	0	0	0	0	0	0	24
31	0	0	0	0	0	1	0	0	1	0	1	1	1	S	1	1	1	1	1	1	1	0	0	1	0	0	1	1	24
HOURLY MAX	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	0	1	1	24
HOURLY AVG	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	24

STATUS FLAG CODES

C	- MONTHLY CALIBRATION	Q	- QUALITY ASSURANCE
C1	- REPEAT CALIBRATION	R	- RECOVERY
Y	- MAINTENANCE	X	- MACHINE MALFUNCTION
S	- DAILY ZERO/SPAN CHECK	G	- OUT FOR REPAIR
S1	- REPEAT ZERO/SPAN CHECK	P	- POWER FAILURE


OBJECTIVE LIMIT:

ALBERTA ENVIRONMENT:	1-HR	172	ppb	24-HR	48	ppb
----------------------	------	-----	-----	-------	----	-----

MONTHLY SUMMARY


NUMBER OF 1-HR EXCEEDANCES:	0		
NUMBER OF 24-HR EXCEEDANCES:	0		
NUMBER OF NON-ZERO READINGS:	116		
MINIMUM 1-HR AVERAGE:	0 ppb @ HOUR ON DAY 1		
MAXIMUM 1-HR AVERAGE:	1 ppb @ HOUR ON DAY 1		
MAXIMUM 24-HR AVERAGE:	1 ppb ON DAY 7		
IZS CALIBRATION TIME:	32 hrs	OPERATIONAL TIME:	743 hrs
MONTHLY CALIBRATION TIME:	3 hrs	AMD OPERATION UPTIME:	99.9 %
STANDARD DEVIATION:	0	MONTHLY AVERAGE:	0 ppb

24 HR AVERAGES October 2018

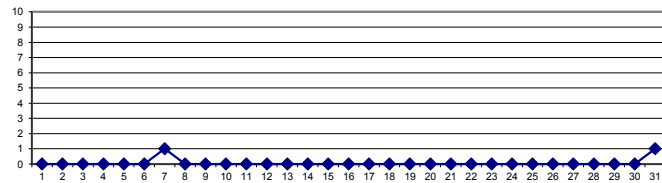



SULPHUR DIOXIDE Hourly Averages (SO<sub>2</sub> ppb)

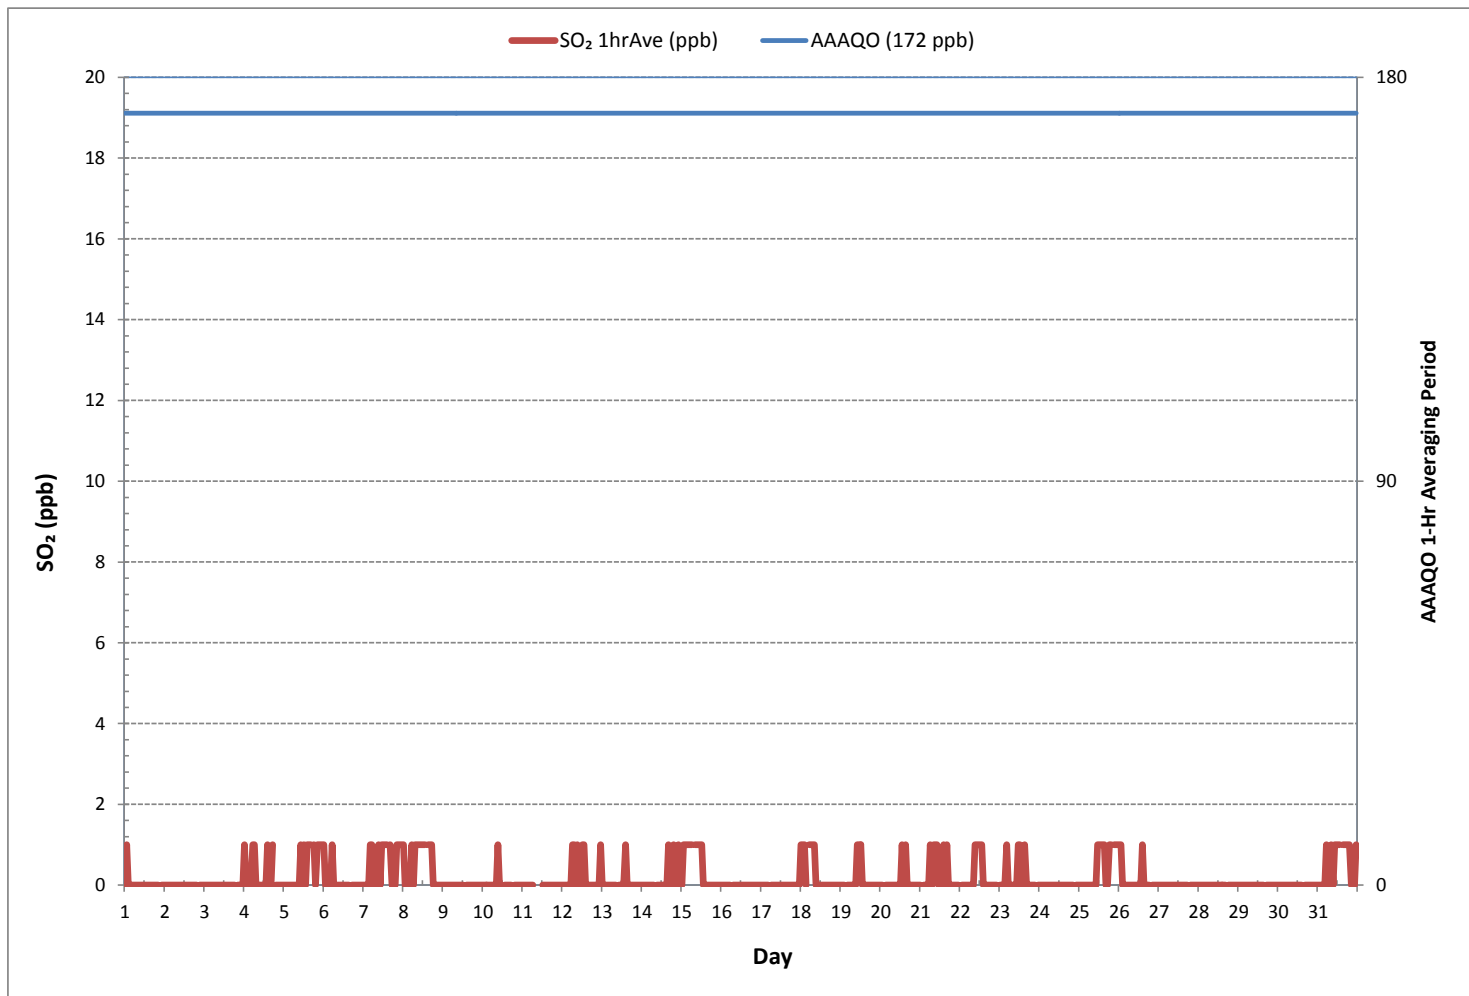

Wind: PRAMP\_986  
 Poll.: PRAMP\_986-SO<sub>2</sub> [ppb]  
 Monthly: 18/10  
 Type: PollutionRose  
 Direction: Blowing From (Wind Frequency)  
 Based On 1 Hr.


Calm: 8.90%

Calm Avg: 0.18 [ppb]


Direction	0-3	3-10	10-85	85-170	>170.0	Total
N	6.9	0.0	0.0	0.0	0.0	6.9
NE	3.3	0.0	0.0	0.0	0.0	3.3
E	12.4	0.0	0.0	0.0	0.0	12.4
SE	18.5	0.0	0.0	0.0	0.0	18.5
S	17.4	0.0	0.0	0.0	0.0	17.4
SW	15.7	0.0	0.0	0.0	0.0	15.7
W	10.2	0.0	0.0	0.0	0.0	10.2
NW	6.8	0.0	0.0	0.0	0.0	6.8
Summary	91.1	0.0	0.0	0.0	0.0	91.1

% Icon Classes (ppb) 91 0-3 0 3-10 0 10-85 0 85-170 0 >170.0

PRAMP\_986 Poll.: PRAMP\_986-SO2[ppb] 2018/10/01 00:00 - 2018/10/31 23:00 Calm: 8.90% Calm Poll Avg: 0.18[ppb]

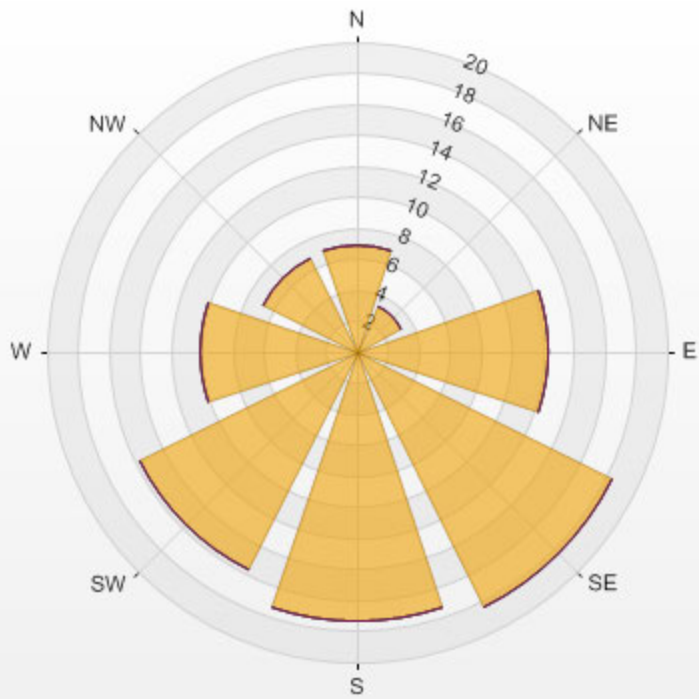

SO2[ppb] Calibration: PRAMP\_986 Monthly: 18/10 Type: Span

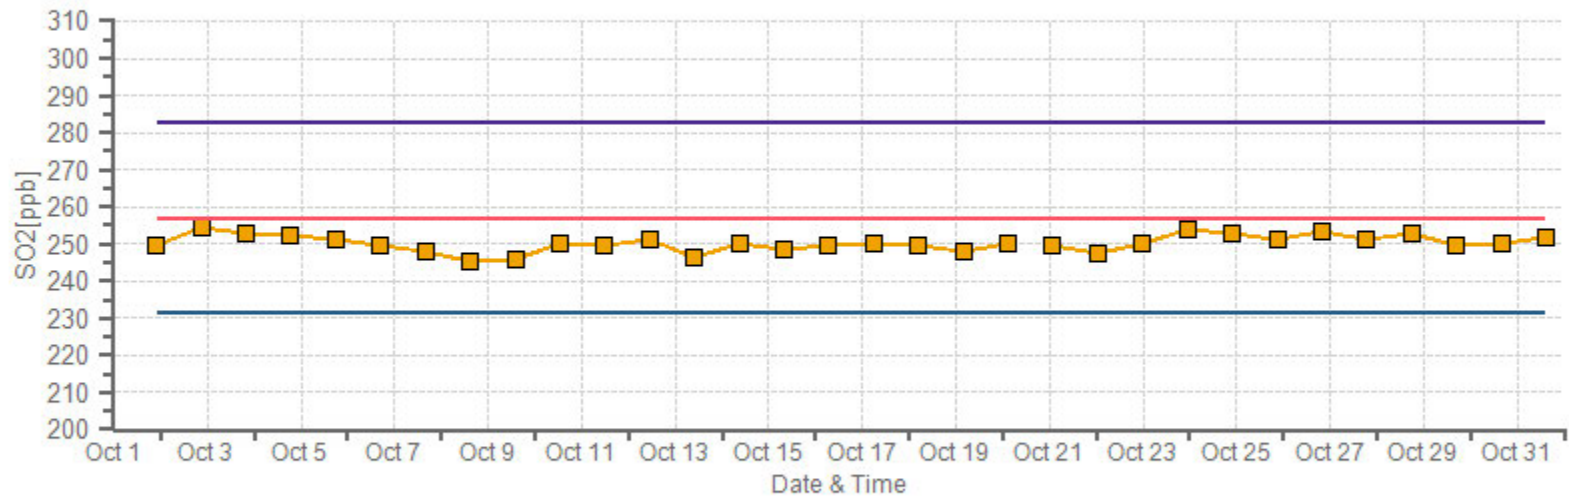

—■— Span Meas — Span Ref — Span Low — Span High

***TOTAL REDUCED SULPHUR***


TOTAL REDUCED SULPHUR Hourly Averages (TRS ppb)

HR START (MST)	0:00	1:00	2:00	3:00	4:00	5:00	6:00	7:00	8:00	9:00	10:00	11:00	12:00	13:00	14:00	15:00	16:00	17:00	18:00	19:00	20:00	21:00	22:00	23:00	DAILY	DAILY	24-HR	RDGS.		
HR END (MST)	0:59	1:59	2:59	3:59	4:59	5:59	6:59	7:59	8:59	9:59	10:59	11:59	12:59	13:59	14:59	15:59	16:59	17:59	18:59	19:59	20:59	21:59	22:59	23:59	MIN.	MAX.	AVG.			
DAY																														
1	0.27	0.25	0.29	0.33	0.30	0.31	0.26	0.27	0.28	0.27	0.24	0.20	0.21	0.19	0.20	0.20	0.19	0.19	0.20	0.20	0.19	S	0.26	0.21	0.19	0.33	0.24	24		
2	0.20	0.21	0.24	0.23	0.21	0.26	0.27	0.22	0.23	0.24	0.23	0.21	0.21	0.21	0.21	0.20	0.21	0.20	0.20	0.20	S	0.27	0.22	0.22	0.20	0.27	0.22	24		
3	0.22	0.21	0.22	0.22	0.19	0.19	0.26	0.23	0.24	0.21	0.21	0.20	0.20	0.20	0.21	0.20	0.20	0.22	0.24	S	0.27	0.23	0.21	0.21	0.19	0.27	0.22	24		
4	0.21	0.20	0.20	0.21	0.20	0.20	0.20	0.20	0.23	0.22	0.21	0.21	0.20	0.23	0.23	0.26	0.20	0.19	S	0.22	0.24	0.22	0.20	0.19	0.19	0.26	0.21	24		
5	0.19	0.21	0.22	0.22	0.21	0.21	0.20	0.20	0.19	0.19	0.18	0.18	0.17	0.16	0.17	0.17	0.18	S	0.22	0.19	0.19	0.19	0.19	0.19	0.19	0.16	0.22	0.19	24	
6	0.19	0.19	0.20	0.20	0.20	0.21	0.21	0.19	0.18	0.20	0.19	0.18	0.19	0.19	0.21	0.21	S	0.23	0.21	0.21	0.22	0.21	0.19	0.19	0.18	0.23	0.20	24		
7	0.20	0.20	0.18	0.21	0.21	0.22	0.23	0.20	0.21	0.21	0.19	0.20	0.21	0.23	0.21	S	0.24	0.20	0.21	0.19	0.21	0.21	0.21	0.22	0.18	0.24	0.21	24		
8	0.22	0.21	0.20	0.21	0.21	0.21	0.21	0.21	0.21	0.21	0.21	0.21	0.22	0.21	S	0.27	0.23	0.22	0.22	0.22	0.21	0.20	0.20	0.21	0.20	0.27	0.21	24		
9	0.19	0.25	0.21	0.21	0.20	0.20	0.20	0.20	0.18	0.20	0.19	0.19	0.20	S	0.25	0.20	0.20	0.20	0.20	0.21	0.20	0.20	0.19	0.19	0.18	0.25	0.20	24		
10	0.18	0.19	0.20	0.20	0.19	0.19	0.19	0.20	0.21	0.21	0.21	0.22	S	0.30	0.27	C	C	C	C	C	C	0.23	0.20	0.18	0.17	0.17	0.30	0.21	24	
11	0.18	0.21	0.21	0.23	0.22	0.21	0.22	0.22	0.21	0.21	0.23	S	0.29	0.26	0.25	0.24	0.26	0.27	0.28	0.27	0.26	0.27	0.26	0.27	0.28	0.29	0.18	0.29	0.24	24
12	0.35	0.42	0.34	0.25	0.23	0.21	0.22	0.22	0.22	0.23	S	0.28	0.25	0.27	0.26	0.27	0.25	0.23	0.28	0.34	0.38	0.39	0.62	0.77	0.21	0.77	0.32	24		
13	0.74	0.39	0.68	0.85	0.61	0.80	0.73	0.63	0.72	S	0.33	0.20	0.21	0.31	0.27	0.23	0.25	0.47	0.53	0.79	0.63	0.46	0.47	0.64	0.20	0.85	0.52	24		
14	0.75	0.57	0.70	0.46	0.43	0.44	0.43	0.37	S	0.41	0.36	0.34	0.30	0.31	0.30	0.29	0.33	0.29	0.26	0.27	0.25	0.25	0.27	0.38	0.25	0.75	0.38	24		
15	0.30	0.29	0.68	1.02	0.80	0.53	1.13	S	0.41	0.41	0.48	0.45	0.29	0.28	0.23	0.23	0.22	0.22	0.21	0.28	1.61	1.69	2.25	1.81	0.21	2.25	0.69	24		
16	1.56	1.30	1.37	1.18	1.06	0.93	S	0.78	0.56	0.54	0.40	0.39	0.35	0.29	0.25	0.25	0.29	0.41	0.42	0.31	0.28	0.26	0.26	0.28	0.25	1.56	0.60	24		
17	0.29	0.29	0.30	0.30	0.32	S	0.32	0.31	0.28	0.30	0.30	0.28	0.26	0.26	0.25	0.25	0.24	0.26	0.26	0.26	0.24	0.23	0.23	0.24	0.23	0.32	0.27	24		
18	0.33	0.42	0.43	0.28	S	0.41	0.49	0.44	0.32	0.26	0.22	0.23	0.37	0.25	0.24	0.22	0.23	0.22	0.23	0.22	0.27	0.40	0.52	0.56	0.22	0.56	0.33	24		
19	0.46	0.40	0.59	S	0.39	0.46	0.54	0.54	0.64	0.45	0.34	0.32	0.26	0.26	0.26	0.26	0.25	0.27	0.31	0.27	0.25	0.26	0.25	0.24	0.24	0.64	0.36	24		
20	0.24	0.24	S	0.30	0.27	0.25	0.27	0.27	0.27	0.25	0.23	0.26	0.30	0.30	0.28	0.25	0.23	0.22	0.23	0.24	0.23	0.23	0.22	0.23	0.22	0.30	0.25	24		
21	0.23	S	0.28	0.26	0.26	0.28	0.24	0.28	0.30	0.33	0.27	0.24	0.23	0.24	0.27	0.24	0.24	0.22	0.26	0.25	0.24	0.25	0.25	0.24	0.22	0.33	0.26	24		
22	S	0.31	0.25	0.25	0.23	0.24	0.25	0.24	0.23	0.24	0.23	0.22	0.23	0.23	0.22	0.24	0.27	0.32	0.32	0.35	0.33	0.27	S	0.22	0.35	0.26	24			
23	0.39	0.32	0.31	0.32	0.32	0.30	0.40	0.38	0.34	0.36	0.30	0.29	0.29	0.29	0.31	0.31	0.31	0.36	0.46	0.44	0.42	0.37	S	0.45	0.29	0.46	0.35	24		
24	0.44	0.38	0.38	0.38	0.37	0.45	0.47	0.41	0.40	0.43	0.34	0.33	0.33	0.32	0.34	0.34	0.35	0.38	0.37	0.37	0.34	S	0.40	0.36	0.32	0.47	0.38	24		
25	0.34	0.38	0.39	0.37	0.32	0.35	0.32	0.31	0.37	0.30	0.27	0.28	0.27	0.28	0.26	0.27	0.27	0.28	0.26	0.25	S	0.30	0.26	0.24	0.24	0.39	0.30	24		
26	0.23	0.25	0.26	0.25	0.24	0.22	0.25	0.22	0.24	0.27	0.23	0.25	0.24	0.23	0.22	0.25	0.25	0.27	0.25	S	0.51	0.32	0.29	0.27	0.22	0.51	0.26	24		
27	0.28	0.27	0.26	0.26	0.25	0.29	0.30	0.27	0.28	0.35	0.34	0.26	0.28	0.32	0.25	0.26	0.27	0.35	S	0.63	0.42	0.50	0.43	0.48	0.25	0.63	0.33	24		
28	0.36	0.36	0.41	0.33	0.39	0.47	0.50	0.49	0.42	0.35	0.33	0.31	0.30	0.23	0.25	0.27	0.26	S	0.30	0.28	0.27	0.73	0.40	0.38	0.23	0.73	0.36	24		
29	0.57	0.45	0.31	0.30	0.31	0.36	0.58	0.53	0.38	0.40	0.34	0.32	0.30	0.29	0.34	0.36	S	0.45	0.35	0.30	0.24	0.36	0.45	0.35	0.24	0.58	0.38	24		
30	0.39	0.45	0.44	0.49	0.42	0.43	0.43	0.40	0.38	0.38	0.28	0.27	0.28	0.27	0.25	S	0.37	0.34	0.34	0.29	0.28	0.27	0.27	0.26	0.25	0.49	0.35	24		
31	0.28	0.27	0.36	0.38	0.37	0.43	0.45	0.41	0.45	0.38	0.30	0.28	0.28	0.27	S	0.37	0.36	0.35	0.28	0.22	0.21	0.24	0.28	0.25	0.21	0.45	0.32	24		
HOURLY MAX	1.56	1.30	1.37	1.18	1.06	0.93	1.13	0.78	0.72	0.54	0.48	0.45	0.37	0.32	0.34	0.37	0.37	0.47	0.53	0.79	1.61	1.69	2.25	1.81						
HOURLY AVG	0.36	0.34	0.37	0.36	0.33	0.34	0.36	0.33	0.32	0.30	0.27	0.26	0.26	0.26	0.25	0.25	0.25	0.28	0.28	0.29	0.33	0.35	0.36	0.36						

STATUS FLAG CODES

C	- MONTHLY CALIBRATION	Q	- QUALITY ASSURANCE
C1	- REPEAT CALIBRATION	R	- RECOVERY
Y	- MAINTENANCE	X	- MACHINE MALFUNCTION
S	- DAILY ZERO/SPAN CHECK	G	- OUT FOR REPAIR
S1	- REPEAT ZERO/SPAN CHECK	P	- POWER FAILURE


24 HR AVERAGES October 2018

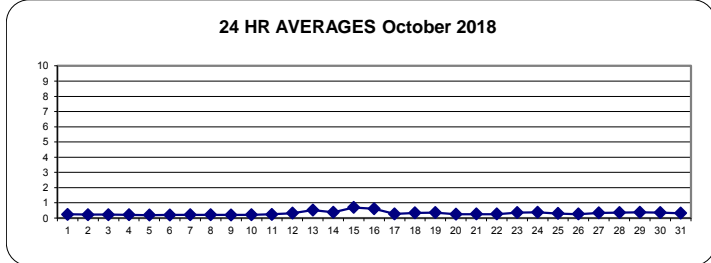

MONTHLY SUMMARY

NUMBER OF NON-ZERO READINGS:	707			
MINIMUM 1-HR AVERAGE:	0.16 ppb	@ HOUR	13	ON DAY 5
MAXIMUM 1-HR AVERAGE:	2.25 ppb	@ HOUR	22	ON DAY 15
MAXIMUM 24-HR AVERAGE:	0.69 ppb			ON DAY 15
IZS CALIBRATION TIME:	32 hrs	OPERATIONAL TIME:	744	hrs
MONTHLY CALIBRATION TIME:	5 hrs	AMD OPERATION UPTIME:	100.0	%
STANDARD DEVIATION:	0.19	MONTHLY AVERAGE:	0.31	ppb

TOTAL REDUCED SULPHUR Hourly Averages (TRS ppb)

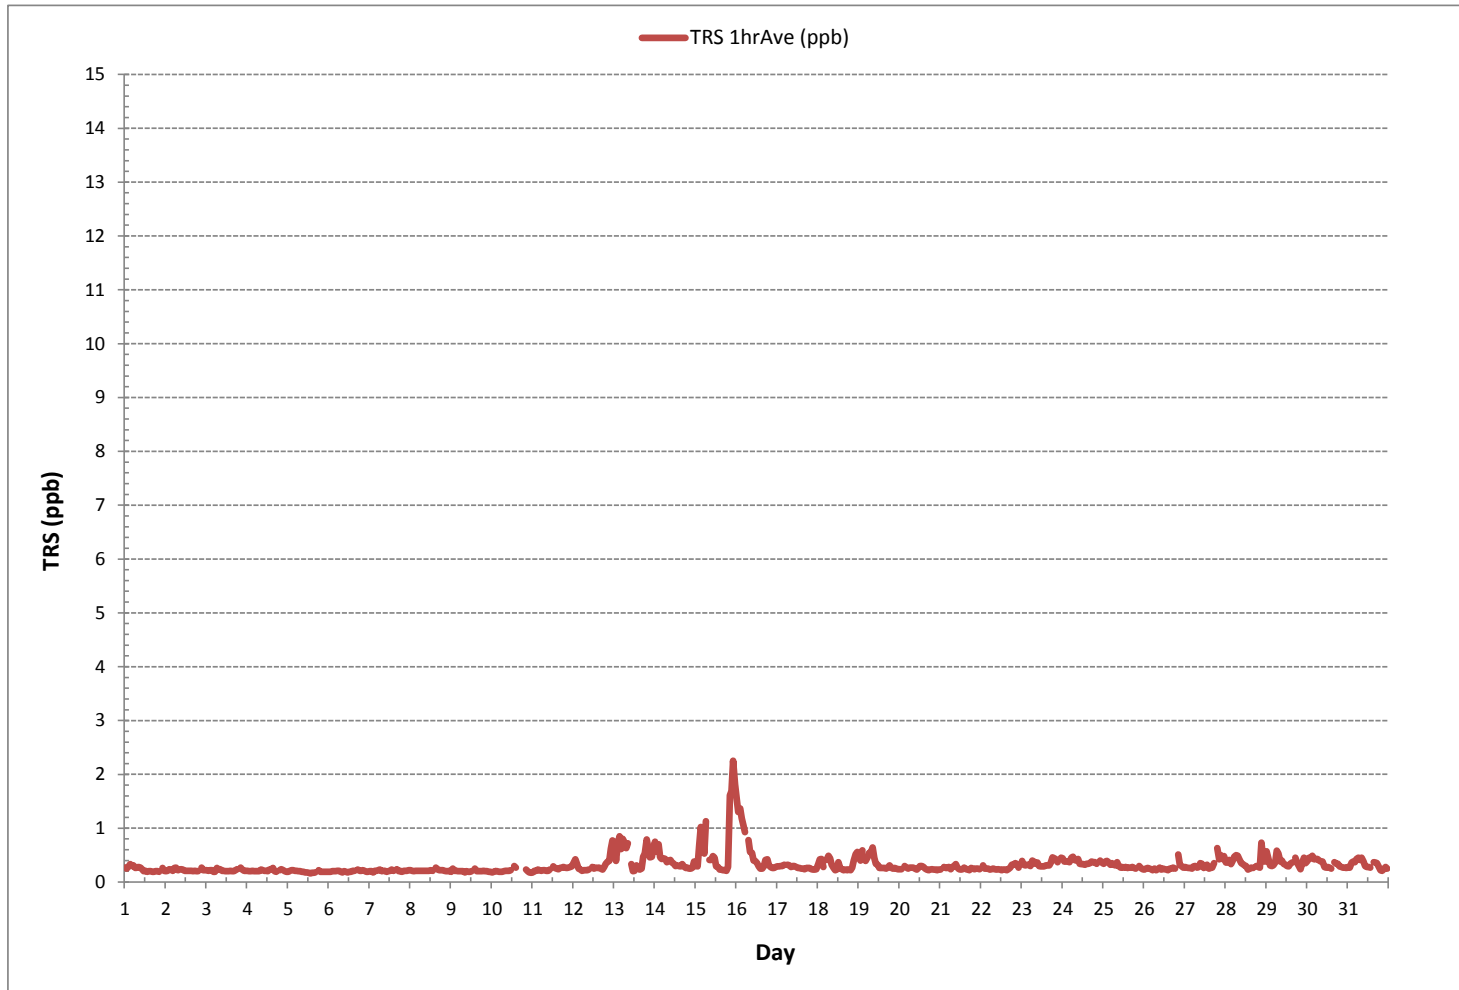

Wind: PRAMP\_986  
Poll.: PRAMP\_986-TRS [ppb]  
Monthly: 18/10  
Type: PollutionRose  
Direction: Blowing From (Wind Frequency)  
Based On 1 Hr.

Calm: 8.91%

Calm Avg: 0.45 [ppb]

Direction	0-1	1-3	3-10	>10.0	Total
N	6.9	0.0	0.0	0.0	6.9
NE	3.3	0.0	0.0	0.0	3.3
E	12.2	0.3	0.0	0.0	12.4
SE	18.0	0.6	0.0	0.0	18.5
S	17.5	0.3	0.0	0.0	17.8
SW	15.6	0.0	0.0	0.0	15.6
W	9.8	0.0	0.0	0.0	9.8
NW	6.8	0.0	0.0	0.0	6.8
Summary	90.0	1.1	0.0	0.0	91.1



% Icon Classes (ppb)


90 0-1

1 1-3

0 3-10

0 >10.0

PRAMP\_986 Poll.: PRAMP\_986-TRS[ppb] 2018/10/01 00:00 - 2018/10/31 23:00 Calm: 8.91% Calm Poll Avg: 0.45[ppb]

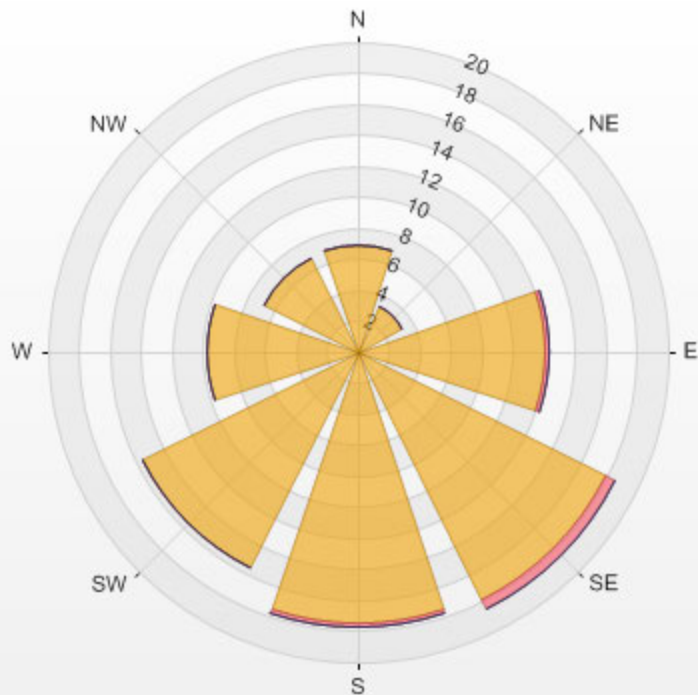

TRS[ppb] Calibration: PRAMP\_986 Monthly: 18/10 Type: Span



■ Span Meas 
 — Span Ref 
 — Span Low 
 — Span High

***TOTAL HYDROCARBON***




TOTAL HYDROCARBONS Hourly Averages (THC ppm)

HR START (MST)	0:00	1:00	2:00	3:00	4:00	5:00	6:00	7:00	8:00	9:00	10:00	11:00	12:00	13:00	14:00	15:00	16:00	17:00	18:00	19:00	20:00	21:00	22:00	23:00	DAILY	DAILY	24-HR	RDGS.
HR END (MST)	0:59	1:59	2:59	3:59	4:59	5:59	6:59	7:59	8:59	9:59	10:59	11:59	12:59	13:59	14:59	15:59	16:59	17:59	18:59	19:59	20:59	21:59	22:59	23:59	MIN.	MAX.	AVG.	
DAY																												
1	2.16	2.22	2.36	2.22	2.17	2.18	2.14	2.14	2.08	Y	2.03	2.02	2.01	2.01	2.00	2.01	2.02	1.99	2.00	2.00	2.00	S	1.99	2.01	1.99	2.36	2.08	23
2	2.01	2.06	2.01	2.00	2.00	2.01	2.06	2.04	2.00	2.01	1.98	1.99	1.98	1.99	1.99	1.99	1.99	1.98	1.98	1.97	S	1.98	1.98	1.99	1.97	2.06	2.00	24
3	2.04	2.42	2.05	2.01	2.00	2.09	2.10	2.06	2.12	2.00	1.99	1.98	1.98	1.99	1.99	1.99	1.99	1.99	1.99	S	1.99	2.00	2.01	2.01	1.98	2.42	2.03	24
4	2.01	2.00	2.00	2.01	2.00	2.00	2.01	2.00	2.01	2.01	2.00	1.99	2.00	2.00	1.99	2.00	2.00	2.00	S	2.00	2.00	2.01	2.01	2.01	1.99	2.01	2.00	24
5	2.00	2.00	2.00	2.00	2.00	1.99	1.99	1.99	1.99	1.99	1.99	1.99	1.99	1.99	1.99	1.99	2.00	S	2.01	2.00	2.02	2.01	2.00	2.02	1.99	2.02	2.00	24
6	2.02	2.00	2.00	2.02	2.01	2.01	2.01	2.01	2.01	2.02	2.02	2.02	2.02	2.02	2.02	2.02	S	2.01	2.01	2.02	2.03	2.03	2.02	2.02	2.00	2.03	2.02	24
7	2.02	2.02	2.02	2.02	2.03	2.03	2.03	2.03	2.03	2.02	2.01	2.01	2.01	2.01	2.01	S	2.00	2.00	2.00	2.01	2.01	2.02	2.03	2.02	2.00	2.03	2.02	24
8	2.02	2.02	2.01	2.01	2.01	2.01	2.01	2.00	2.00	2.01	2.01	2.00	2.00	2.00	S	2.01	2.01	2.00	1.99	2.02	2.02	2.03	2.02	1.99	2.03	2.02	24	
9	2.02	2.11	2.03	2.01	2.01	2.01	2.01	2.01	2.00	2.01	2.00	2.00	S	2.01	2.01	2.01	2.01	2.01	2.01	2.05	2.06	2.03	2.02	2.01	2.00	2.11	2.02	24
10	2.01	2.02	2.01	2.01	2.01	2.02	2.02	2.02	2.03	2.04	2.06	2.04	S	2.05	2.06	C	C	C	C	2.02	2.02	2.02	2.03	2.04	2.01	2.06	2.03	24
11	2.04	2.04	2.03	2.03	2.02	2.02	2.01	1.99	1.99	1.98	1.99	S	1.99	1.99	1.97	1.95	1.96	1.97	1.98	1.97	1.95	1.95	1.94	1.93	1.93	2.04	1.99	24
12	1.94	1.95	1.95	1.95	1.95	1.95	1.96	1.96	1.97	1.98	S	1.98	1.98	1.97	1.98	1.99	1.98	1.97	2.10	2.13	2.13	1.99	2.03	1.97	1.94	2.13	1.99	24
13	2.09	2.02	1.98	1.98	1.99	2.00	2.00	2.02	2.04	S	1.98	1.97	1.96	1.95	1.95	1.95	1.95	1.95	1.95	1.95	1.97	1.97	1.97	1.98	1.95	2.09	1.98	24
14	1.98	1.98	1.98	1.98	1.98	1.97	1.97	1.97	S	1.97	1.97	1.96	1.94	1.93	1.92	1.92	1.92	1.92	1.93	1.93	1.92	1.92	1.92	1.92	1.92	1.98	1.95	24
15	2.02	2.00	1.95	1.92	1.93	1.93	S	1.93	1.93	1.94	1.94	1.94	1.95	1.96	1.97	1.93	1.96	1.96	2.03	1.93	2.11	1.94	1.94	1.92	2.11	1.96	24	
16	1.95	1.99	1.99	2.02	2.03	2.01	S	2.00	1.97	1.96	1.96	1.95	1.95	1.95	1.95	1.94	1.94	1.93	1.95	1.95	1.95	1.94	1.94	1.93	2.03	1.96	24	
17	1.93	1.93	1.93	1.93	1.92	S	1.92	1.93	1.94	1.96	1.96	1.96	1.95	1.95	1.93	1.92	1.92	1.92	1.91	1.92	1.93	1.92	1.92	1.92	1.91	1.96	1.93	24
18	1.92	1.92	1.92	1.94	S	1.93	1.95	1.99	2.00	1.99	1.95	1.96	1.95	1.94	1.96	1.96	1.96	2.02	2.12	2.09	2.01	2.00	2.02	1.99	1.92	2.12	1.98	24
19	1.98	1.98	2.00	S	2.05	2.05	2.06	2.05	2.09	2.06	2.02	2.00	1.98	1.96	1.95	1.94	1.94	1.95	1.98	1.97	1.94	1.95	1.96	1.96	1.94	2.09	1.99	24
20	1.95	1.95	S	1.97	1.96	1.96	1.96	1.95	1.94	1.94	1.93	1.94	1.96	1.95	1.96	1.94	1.93	1.93	1.94	1.94	1.95	1.95	1.95	1.93	1.97	1.95	24	
21	1.95	S	1.96	1.96	1.97	1.96	1.97	1.98	2.04	1.98	1.99	2.00	1.99	1.98	1.96	1.96	1.94	1.95	1.96	1.97	1.98	1.99	2.00	2.04	1.94	2.04	1.98	24
22	S	2.07	2.09	2.04	2.02	2.00	1.99	2.01	2.08	2.06	1.97	1.96	1.96	1.96	1.94	1.95	1.98	1.98	2.00	2.03	2.06	2.05	S	1.94	2.09	2.01	24	
23	2.05	2.06	2.08	2.08	2.04	2.09	2.11	2.16	2.11	2.09	2.06	2.06	2.06	2.08	2.08	2.08	2.20	2.15	2.09	2.09	2.11	2.12	S	2.14	2.04	2.20	2.10	24
24	2.18	2.15	2.18	2.16	2.15	2.24	2.30	2.39	2.45	2.37	2.12	2.08	2.05	2.04	2.05	2.04	2.05	2.06	2.07	2.08	2.09	S	2.06	2.06	2.04	2.45	2.15	24
25	2.08	2.11	2.09	2.07	2.08	2.05	2.02	2.02	2.02	1.99	1.98	1.96	1.95	1.94	1.93	1.93	1.94	1.93	1.94	1.93	S	1.92	1.93	1.93	1.92	2.11	1.99	24
26	1.93	1.94	1.95	1.96	1.95	1.96	1.96	1.95	1.96	1.97	1.96	1.94	1.94	1.93	1.92	1.92	1.93	1.95	1.95	S	1.96	1.96	1.97	1.98	1.92	1.98	1.95	24
27	1.98	1.98	1.96	1.94	1.94	1.95	1.95	1.95	1.94	1.95	1.95	1.95	1.96	1.95	1.94	1.95	2.04	1.95	S	1.95	1.95	1.96	1.96	1.98	1.94	2.04	1.96	24
28	2.00	2.02	2.05	2.04	2.05	2.10	2.05	2.03	2.02	2.00	1.98	1.96	1.96	1.95	1.94	1.94	S	1.95	2.03	2.40	2.08	2.00	2.02	1.94	2.40	2.02	24	
29	2.01	1.98	1.99	1.98	1.98	1.98	1.98	2.06	2.03	2.04	2.04	2.03	2.01	1.99	1.99	1.99	S	1.98	1.99	1.98	1.99	1.99	2.02	1.98	2.06	2.00	24	
30	2.02	2.04	2.03	2.04	2.02	2.00	2.00	1.99	2.00	2.00	1.99	1.97	1.96	1.95	S	1.93	1.95	1.96	1.97	1.96	1.96	1.95	1.96	1.93	2.04	1.98	24	
31	1.96	1.96	1.97	1.97	1.97	1.99	2.00	1.98	1.97	1.97	1.97	1.97	1.95	1.95	S	2.00	2.03	2.00	1.98	1.98	1.99	2.00	2.00	2.00	1.95	2.03	1.98	24
HOURLY MAX	2.18	2.42	2.36	2.22	2.17	2.24	2.30	2.39	2.45	2.37	2.12	2.08	2.06	2.08	2.08	2.20	2.15	2.12	2.13	2.40	2.12	2.06	2.14					
HOURLY AVG	2.01	2.03	2.02	2.01	2.01	2.02	2.02	2.02	2.03	2.01	1.99	1.99	1.98	1.98	1.98	1.97	1.98	1.98	1.99	2.00	2.01	2.00	1.99	1.99				

STATUS FLAG CODES

C	- MONTHLY CALIBRATION	Q	- QUALITY ASSURANCE
C1	- REPEAT CALIBRATION	R	- RECOVERY
Y	- MAINTENANCE	X	- MACHINE MALFUNCTION
S	- DAILY ZERO/SPAN CHECK	G	- OUT FOR REPAIR
S1	- REPEAT ZERO/SPAN CHECK	P	- POWER FAILURE


24 HR AVERAGES October 2018

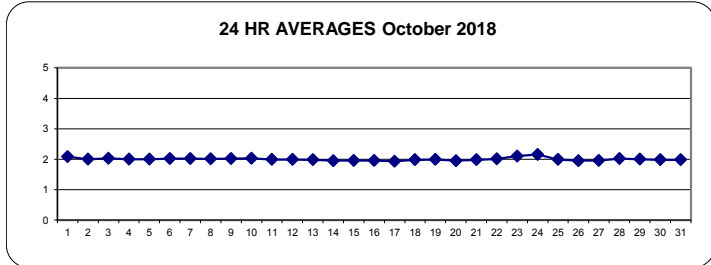

MONTHLY SUMMARY

NUMBER OF NON-ZERO READINGS:	707			
MINIMUM 1-HR AVERAGE:	1.91 ppm	@ HOUR	17	ON DAY 17
MAXIMUM 1-HR AVERAGE:	2.45 ppm	@ HOUR	8	ON DAY 24
MAXIMUM 24-HR AVERAGE:	2.15 ppm			ON DAY 24
IZS CALIBRATION TIME:	32 hrs	OPERATIONAL TIME:	743 hrs	
MONTHLY CALIBRATION TIME:	4 hrs	AMD OPERATION UPTIME:	99.9 %	
STANDARD DEVIATION:	0.06	MONTHLY AVERAGE:	2.00 ppm	

TOTAL HYDROCARBONS Hourly Averages (THC ppm)

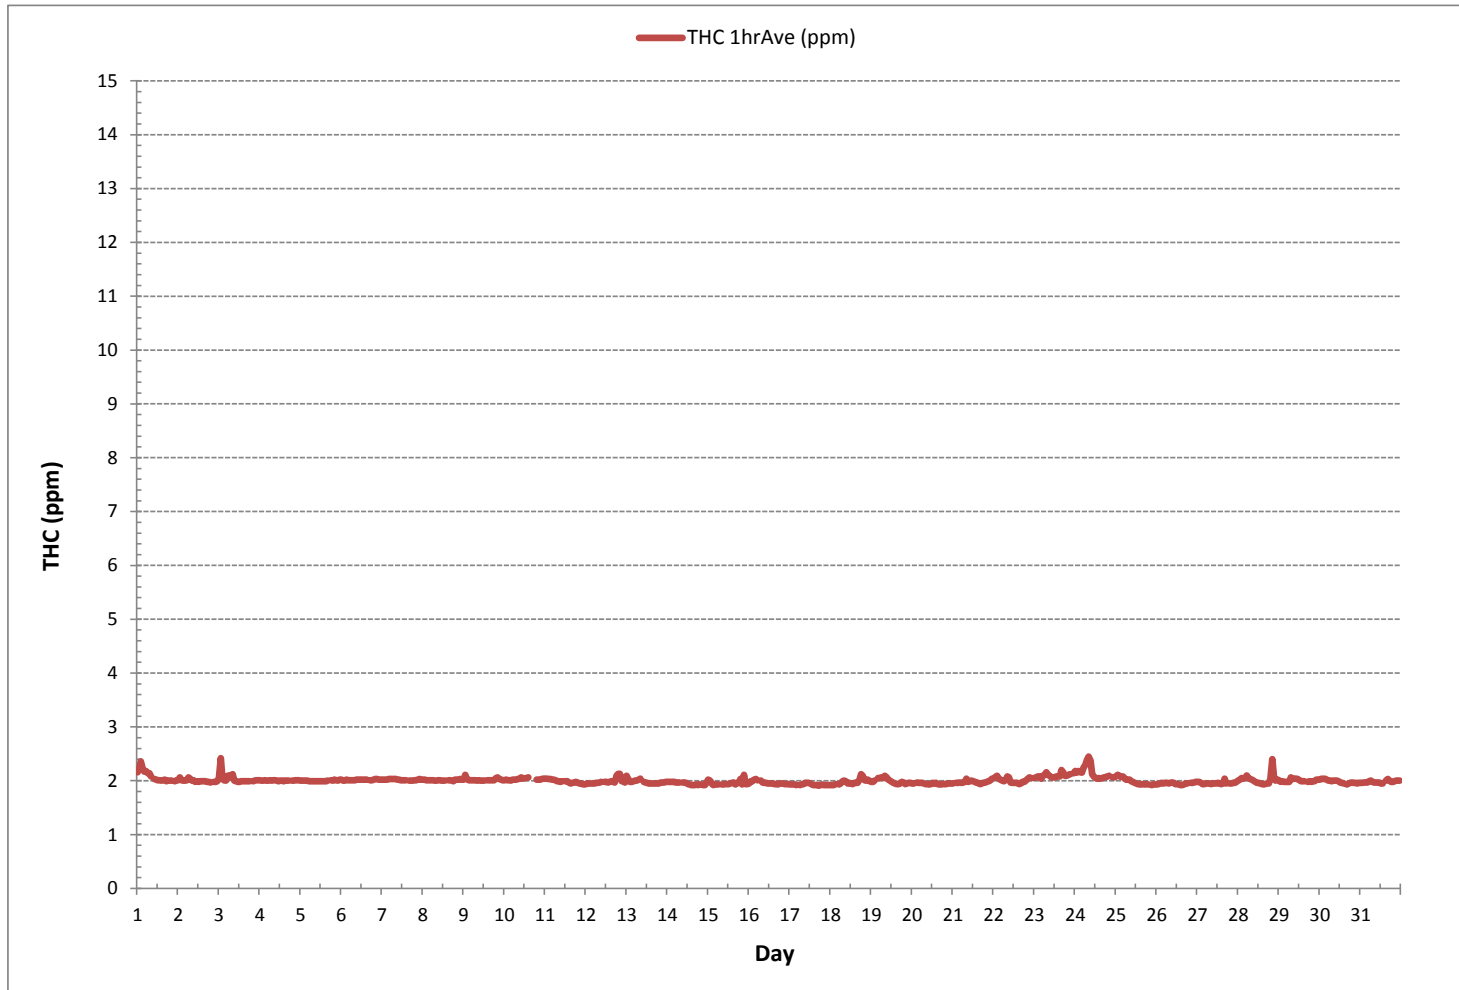

Wind: PRAMP\_986  
 Poll.: PRAMP\_986-THC55 [ppm]  
 Monthly: 18/10  
 Type: PollutionRose  
 Direction: Blowing From (Wind Frequency)  
 Based On 1 Hr.


Calm: 8.91%

Calm Avg: 2.06 [ppm]

Direction	0-2	2-3	3-5	5-10	>10.0	Total
N	4.0	3.0	0.0	0.0	0.0	6.9
NE	0.7	2.6	0.0	0.0	0.0	3.3
E	2.6	9.9	0.0	0.0	0.0	12.5
SE	6.1	12.5	0.0	0.0	0.0	18.5
S	14.0	3.8	0.0	0.0	0.0	17.8
SW	13.6	2.1	0.0	0.0	0.0	15.7
W	8.6	1.1	0.0	0.0	0.0	9.8
NW	4.4	2.3	0.0	0.0	0.0	6.6
<b>Summary</b>	53.9	37.2	0.0	0.0	0.0	91.1

% Icon Classes (ppm) 54 0-2 37 2-3 0 3-5 0 5-10 0 >10.0

PRAMP\_986 Poll.: PRAMP\_986-THC55[ppm] 2018/10/01 00:00 - 2018/10/31 23:00 Calm: 8.91% Calm Poll Avg: 2.06[ppm]

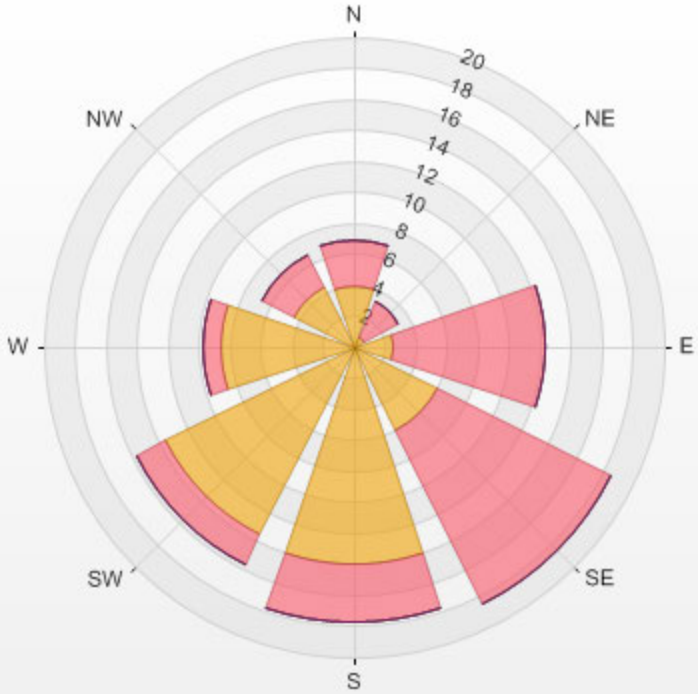

THC55[ppm] Calibration: PRAMP\_986 Monthly: 18/10 Type: Span



—■— Span Meas — Span Ref — Span Low — Span High



***METHANE***




METHANE Hourly Averages (CH<sub>4</sub> ppm)

HR START (MST)	0:00	1:00	2:00	3:00	4:00	5:00	6:00	7:00	8:00	9:00	10:00	11:00	12:00	13:00	14:00	15:00	16:00	17:00	18:00	19:00	20:00	21:00	22:00	23:00	DAILY	DAILY	24-HR	RDGS.	
HR END (MST)	0:59	1:59	2:59	3:59	4:59	5:59	6:59	7:59	8:59	9:59	10:59	11:59	12:59	13:59	14:59	15:59	16:59	17:59	18:59	19:59	20:59	21:59	22:59	23:59	MIN.	MAX.	AVG.		
DAY																													
1	2.16	2.22	2.36	2.22	2.17	2.18	2.14	2.14	2.08	Y	2.03	2.02	2.01	2.01	2.00	2.01	2.02	1.99	2.00	2.00	2.00	S	1.99	2.01	1.99	2.36	2.08	23	
2	2.01	2.06	2.01	2.00	2.00	2.01	2.06	2.04	2.00	2.01	1.98	1.99	1.98	1.99	1.99	1.99	1.99	1.98	1.98	1.97	S	1.98	1.98	1.99	1.97	2.06	2.00	24	
3	2.04	2.42	2.05	2.01	2.00	2.09	2.10	2.06	2.12	2.00	1.99	1.98	1.98	1.99	1.99	1.99	1.99	1.99	1.99	S	1.99	2.00	2.01	2.01	1.98	2.42	2.03	24	
4	2.01	2.00	2.00	2.01	2.00	2.00	2.01	2.00	2.01	2.01	2.00	1.99	2.00	2.00	1.99	2.00	2.00	S	2.00	2.00	2.01	2.01	2.01	2.01	1.99	2.01	2.00	24	
5	2.00	2.00	2.00	2.00	2.00	1.99	1.99	1.99	1.99	1.99	1.99	1.99	1.99	1.99	1.99	2.00	S	2.01	2.00	2.02	2.01	2.00	2.02	2.00	1.99	2.02	2.00	24	
6	2.02	2.00	2.00	2.02	2.01	2.01	2.01	2.01	2.01	2.02	2.02	2.02	2.02	2.02	2.02	S	2.01	2.01	2.02	2.03	2.03	2.02	2.02	2.02	2.00	2.03	2.02	24	
7	2.02	2.02	2.02	2.02	2.03	2.03	2.03	2.03	2.03	2.02	2.01	2.01	2.01	2.01	S	2.00	2.00	2.00	2.01	2.01	2.02	2.03	2.02	2.00	2.03	2.02	24		
8	2.02	2.02	2.01	2.01	2.01	2.01	2.00	2.00	2.01	2.01	2.00	2.00	2.00	S	2.01	2.01	2.00	1.99	2.02	2.02	2.03	2.02	1.99	2.03	2.02	1.99	2.03	24	
9	2.02	2.11	2.03	2.01	2.01	2.01	2.01	2.01	2.00	2.01	2.00	2.00	S	2.01	2.01	2.01	2.01	2.01	2.01	2.05	2.06	2.03	2.02	2.01	2.00	2.11	2.02	24	
10	2.01	2.02	2.01	2.01	2.01	2.02	2.02	2.02	2.03	2.04	2.06	2.04	S	2.05	2.06	C	C	C	C	2.02	2.02	2.02	2.03	2.04	2.01	2.06	2.03	24	
11	2.04	2.04	2.03	2.03	2.02	2.01	1.99	1.99	1.98	1.99	S	1.99	1.99	1.97	1.95	1.96	1.97	1.98	1.97	1.95	1.95	1.94	1.93	1.93	2.04	2.06	2.03	24	
12	1.94	1.95	1.95	1.95	1.95	1.95	1.96	1.96	1.97	1.98	S	1.98	1.98	1.97	1.98	1.99	1.98	1.97	2.10	2.13	2.13	1.99	2.03	1.97	1.94	2.13	1.99	24	
13	2.09	2.02	1.98	1.98	1.99	2.00	2.00	2.02	2.04	S	1.98	1.97	1.96	1.95	1.95	1.95	1.95	1.95	1.95	1.95	1.95	1.97	1.97	1.98	1.95	2.09	1.98	24	
14	1.98	1.98	1.98	1.98	1.98	1.97	1.97	1.97	S	1.97	1.97	1.96	1.94	1.93	1.92	1.92	1.92	1.93	1.93	1.92	1.92	1.92	1.92	1.92	1.92	1.98	1.95	24	
15	2.02	2.00	1.95	1.92	1.93	1.93	S	1.93	1.93	1.92	1.94	1.94	1.95	1.96	1.97	1.93	1.96	1.96	2.03	1.93	2.11	1.94	1.94	1.92	2.11	1.96	24		
16	1.95	1.99	1.99	2.02	2.03	2.01	S	2.00	1.97	1.96	1.96	1.95	1.95	1.95	1.95	1.94	1.94	1.93	1.95	1.95	1.95	1.94	1.94	1.93	2.03	1.96	24		
17	1.93	1.93	1.93	1.93	1.92	S	1.92	1.93	1.94	1.96	1.96	1.96	1.95	1.93	1.92	1.92	1.92	1.92	1.92	1.92	1.92	1.92	1.92	1.92	1.92	1.91	1.96	24	
18	1.92	1.92	1.92	1.94	S	1.93	1.95	1.99	2.00	1.99	1.95	1.96	1.95	1.94	1.96	1.96	1.96	2.02	2.12	2.09	2.01	2.00	2.02	1.99	1.92	2.12	1.98	24	
19	1.98	1.98	2.00	S	2.05	2.05	2.06	2.05	2.09	2.06	2.02	2.00	1.98	1.96	1.95	1.94	1.94	1.95	1.98	1.97	1.94	1.95	1.96	1.96	1.94	2.09	1.99	24	
20	1.95	1.95	S	1.97	1.96	1.96	1.96	1.95	1.94	1.94	1.93	1.94	1.96	1.95	1.96	1.94	1.93	1.93	1.94	1.94	1.95	1.95	1.93	1.97	1.95	1.97	1.95	24	
21	1.95	S	1.96	1.96	1.97	1.96	1.97	1.98	2.04	1.98	1.99	2.00	1.99	1.98	1.96	1.96	1.94	1.95	1.96	1.97	1.98	1.99	2.00	2.04	1.94	2.04	1.98	24	
22	S	2.07	2.09	2.04	2.02	2.00	1.99	2.01	2.08	2.06	1.97	1.96	1.96	1.96	1.94	1.95	1.98	1.98	2.00	2.03	2.06	2.05	S	1.94	2.09	2.01	24		
23	2.05	2.06	2.08	2.08	2.04	2.09	2.11	2.16	2.11	2.09	2.06	2.06	2.06	2.08	2.08	2.08	2.20	2.15	2.09	2.09	2.11	2.12	S	2.14	2.04	2.20	2.10	24	
24	2.18	2.15	2.18	2.16	2.15	2.24	2.30	2.39	2.44	2.37	2.12	2.08	2.05	2.04	2.05	2.04	2.05	2.06	2.07	2.08	2.09	S	2.06	2.06	2.04	2.44	2.15	24	
25	2.08	2.11	2.09	2.07	2.08	2.05	2.02	2.02	2.02	1.99	1.98	1.96	1.95	1.94	1.93	1.93	1.94	1.93	1.94	1.93	1.93	S	1.92	1.93	1.93	1.92	2.11	1.99	24
26	1.93	1.94	1.95	1.96	1.95	1.96	1.96	1.95	1.96	1.97	1.96	1.94	1.94	1.93	1.92	1.92	1.93	1.95	1.95	S	1.96	1.96	1.97	1.98	1.92	1.98	1.95	24	
27	1.98	1.98	1.96	1.94	1.94	1.95	1.95	1.95	1.94	1.95	1.95	1.95	1.96	1.95	1.94	1.95	2.04	1.95	S	1.95	1.95	1.96	1.96	1.98	1.94	2.04	1.96	24	
28	2.00	2.02	2.05	2.04	2.05	2.10	2.05	2.03	2.02	2.00	1.98	1.96	1.96	1.95	1.94	1.94	S	1.95	2.03	2.40	2.08	2.00	2.02	1.94	2.40	2.02	24		
29	2.01	1.98	1.99	1.98	1.98	1.98	1.98	2.06	2.03	2.04	2.04	2.03	2.01	1.99	1.99	1.99	S	1.98	1.99	1.98	1.99	1.99	2.02	1.98	2.06	2.00	24		
30	2.02	2.04	2.03	2.04	2.02	2.00	2.00	1.99	2.00	2.00	1.99	1.97	1.96	1.95	S	1.93	1.95	1.96	1.97	1.96	1.96	1.95	1.96	1.93	2.04	1.98	24		
31	1.96	1.96	1.97	1.97	1.97	1.99	2.00	1.98	1.97	1.97	1.97	1.97	1.95	1.95	S	2.00	2.03	2.00	1.98	1.98	1.99	2.00	2.00	2.00	1.95	2.03	1.98	24	
HOURLY MAX	2.18	2.42	2.36	2.22	2.17	2.24	2.30	2.39	2.44	2.37	2.12	2.08	2.06	2.08	2.08	2.08	2.20	2.15	2.12	2.13	2.40	2.12	2.06	2.14					
HOURLY AVG	2.01	2.03	2.02	2.01	2.01	2.02	2.02	2.02	2.03	2.01	1.99	1.99	1.98	1.98	1.98	1.97	1.98	1.98	1.99	2.00	2.01	2.00	1.99	1.99					

STATUS FLAG CODES

C	- MONTHLY CALIBRATION	Q	- QUALITY ASSURANCE
C1	- REPEAT CALIBRATION	R	- RECOVERY
Y	- MAINTENANCE	X	- MACHINE MALFUNCTION
S	- DAILY ZERO/SPAN CHECK	G	- OUT FOR REPAIR
S1	- REPEAT ZERO/SPAN CHECK	P	- POWER FAILURE


24 HR AVERAGES October 2018

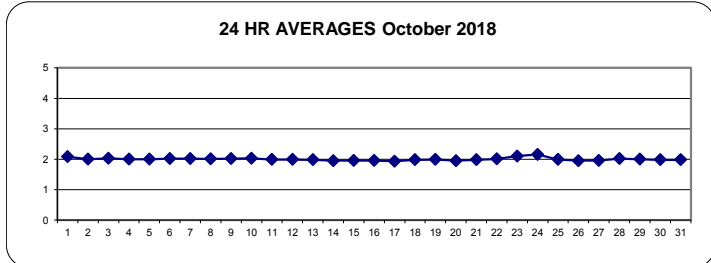

MONTHLY SUMMARY

NUMBER OF NON-ZERO READINGS:	707			
MINIMUM 1-HR AVERAGE:	1.91 ppm	@ HOUR	17	ON DAY 17
MAXIMUM 1-HR AVERAGE:	2.44 ppm	@ HOUR	8	ON DAY 24
MAXIMUM 24-HR AVERAGE:	2.15 ppm			ON DAY 24
IZS CALIBRATION TIME:	32 hrs	OPERATIONAL TIME:	743 hrs	
MONTHLY CALIBRATION TIME:	4 hrs	AMD OPERATION UPTIME:	99.9 %	
STANDARD DEVIATION:	0.06	MONTHLY AVERAGE:	2.00 ppm	

METHANE Hourly Averages (CH<sub>4</sub> ppm)

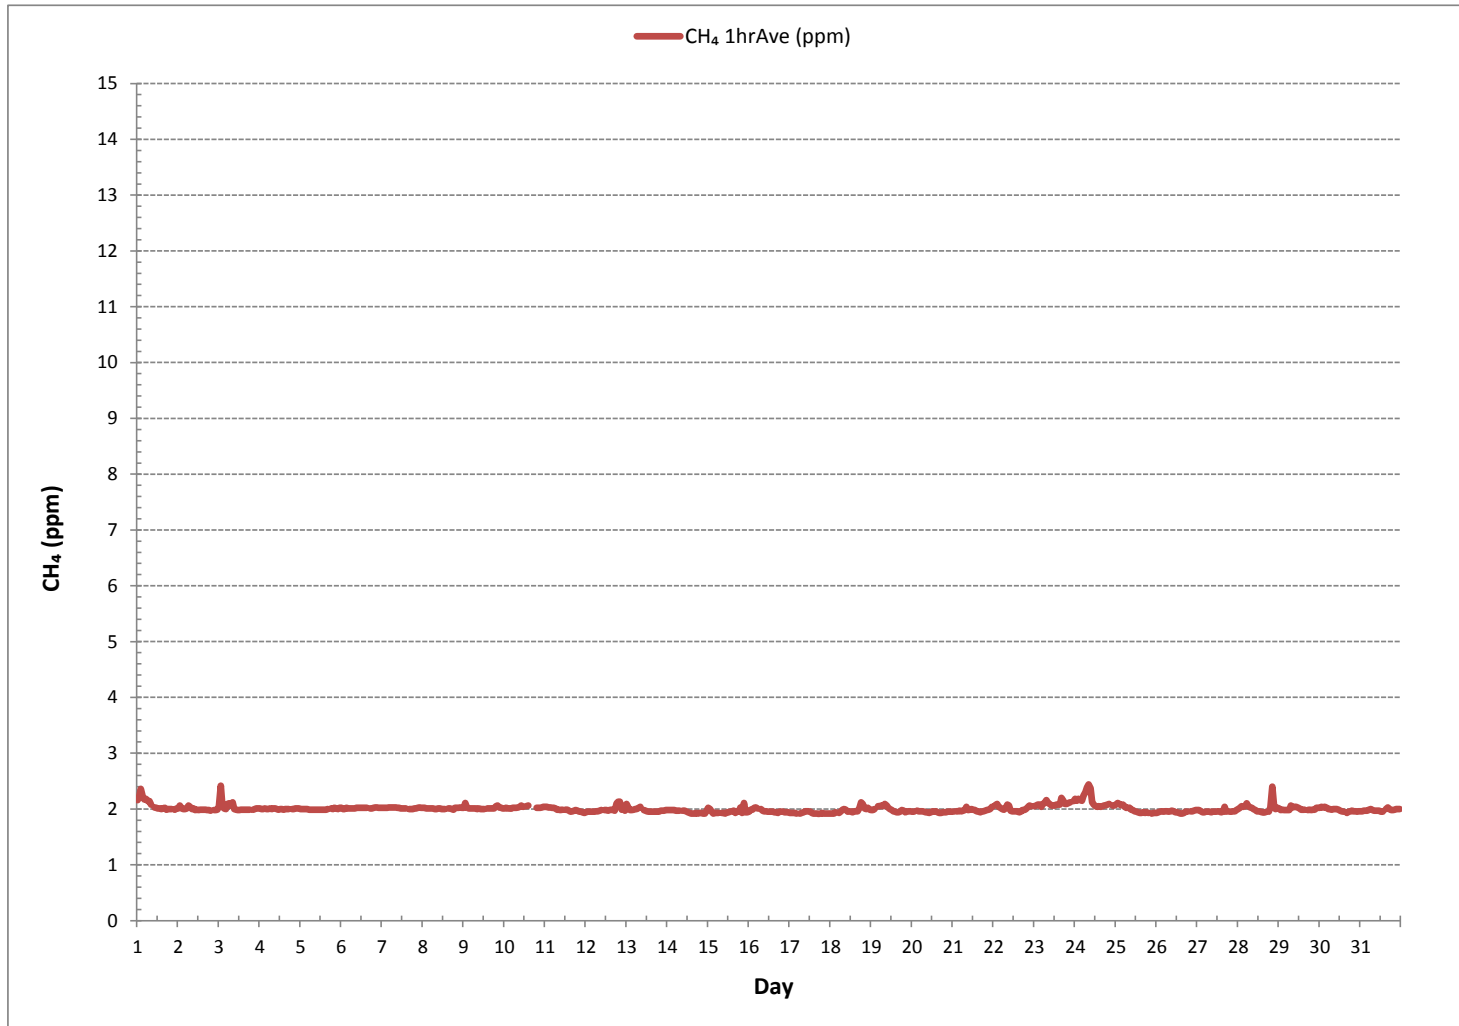

Wind: PRAMP\_986  
 Poll.: PRAMP\_986-CH<sub>4</sub> [ppm]  
 Monthly: 18/10  
 Type: PollutionRose  
 Direction: Blowing From (Wind Frequency)  
 Based On 1 Hr.

Calm: 8.91%

Calm Avg: 2.06 [ppm]

Direction	0-2	2-3	3-5	5-10	>10.0	Total
N	4.0	3.0	0.0	0.0	0.0	6.9
NE	0.7	2.6	0.0	0.0	0.0	3.3
E	2.6	9.9	0.0	0.0	0.0	12.5
SE	6.1	12.5	0.0	0.0	0.0	18.5
S	14.0	3.8	0.0	0.0	0.0	17.8
SW	13.6	2.1	0.0	0.0	0.0	15.7
W	8.6	1.1	0.0	0.0	0.0	9.8
NW	4.4	2.3	0.0	0.0	0.0	6.6
<b>Summary</b>	53.9	37.2	0.0	0.0	0.0	91.1

% Icon Classes (ppm)

54 0-2


37 2-3

0 3-5

0 5-10

0 >10.0

PRAMP\_986 Poll.: PRAMP\_986-CH4[ppm] 2018/10/01 00:00 - 2018/10/31 23:00 Calm: 8.91% Calm Poll Avg: 2.06[ppm]

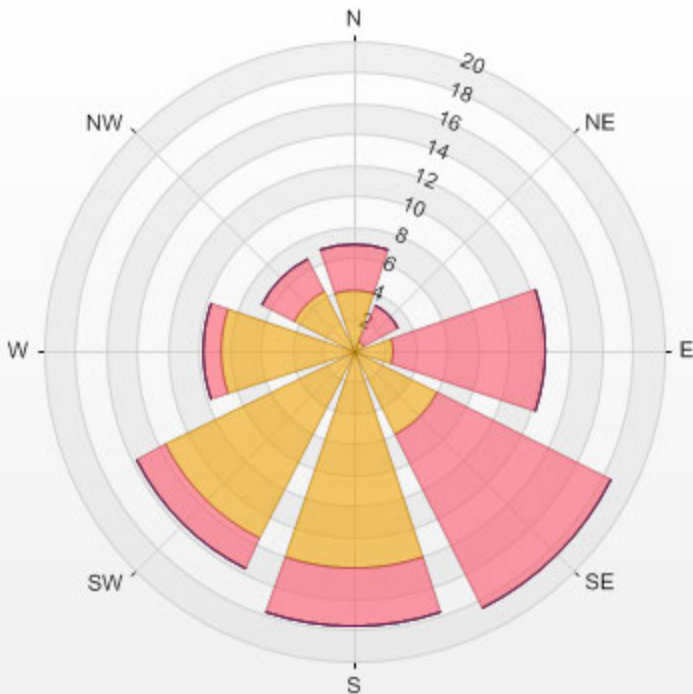

CH4[ppm] Calibration: PRAMP\_986 Monthly: 18/10 Type: Span



—■— Span Meas — Span Ref — Span Low — Span High

***NON-METHANE HYDROCARBON***




NON-METHANE HYDROCARBONS Hourly Averages (NMHC ppm)

HR START (MST)	0:00	1:00	2:00	3:00	4:00	5:00	6:00	7:00	8:00	9:00	10:00	11:00	12:00	13:00	14:00	15:00	16:00	17:00	18:00	19:00	20:00	21:00	22:00	23:00	DAILY	DAILY	24-HR	RDGS.
HR END (MST)	0:59	1:59	2:59	3:59	4:59	5:59	6:59	7:59	8:59	9:59	10:59	11:59	12:59	13:59	14:59	15:59	16:59	17:59	18:59	19:59	20:59	21:59	22:59	23:59	MIN.	MAX.	AVG.	
DAY																												
1	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	Y	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	23
2	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	24
3	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	24	
4	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	24		
5	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	24		
6	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24		
7	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24		
8	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24		
9	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24		
10	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	C	C	C	C	0.00	0.00	0.00	0.00	0.00	0.00	24		
11	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24		
12	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24		
13	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24		
14	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24		
15	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.01	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.01	0.00	24		
16	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24		
17	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24		
18	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24		
19	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24		
20	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24		
21	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24		
22	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	24		
23	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	24		
24	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.01	0.01	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.01	0.00	24		
25	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	24			
26	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	24			
27	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	24			
28	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24			
29	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24			
30	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24			
31	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24			
HOURLY MAX	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.01	0.01	0.00	0.01	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00		
HOURLY AVG	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00		

STATUS FLAG CODES

C	- MONTHLY CALIBRATION	Q	- QUALITY ASSURANCE
C1	- REPEAT CALIBRATION	R	- RECOVERY
Y	- MAINTENANCE	X	- MACHINE MALFUNCTION
S	- DAILY ZERO/SPAN CHECK	G	- OUT FOR REPAIR
S1	- REPEAT ZERO/SPAN CHECK	P	- POWER FAILURE

24 HR AVERAGES October 2018

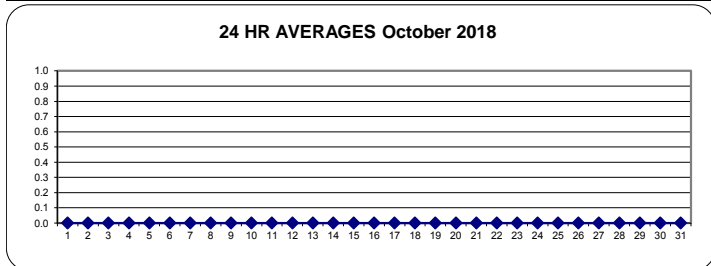


MONTHLY SUMMARY

NUMBER OF NON-ZERO READINGS:	3
MINIMUM 1-HR AVERAGE:	0.00 ppm @ HOUR 0 ON DAY 1
MAXIMUM 1-HR AVERAGE:	0.01 ppm @ HOUR 10 ON DAY 15
MAXIMUM 24-HR AVERAGE:	0.00 ppm ON DAY 1
IZS CALIBRATION TIME:	32 hrs OPERATIONAL TIME: 743 hrs
MONTHLY CALIBRATION TIME:	4 hrs AMD OPERATION UPTIME: 99.9 %
STANDARD DEVIATION:	0.00 MONTHLY AVERAGE: 0.00 ppm





NON-METHANE HYDROCARBONS Hourly Averages (NMHC ppm)

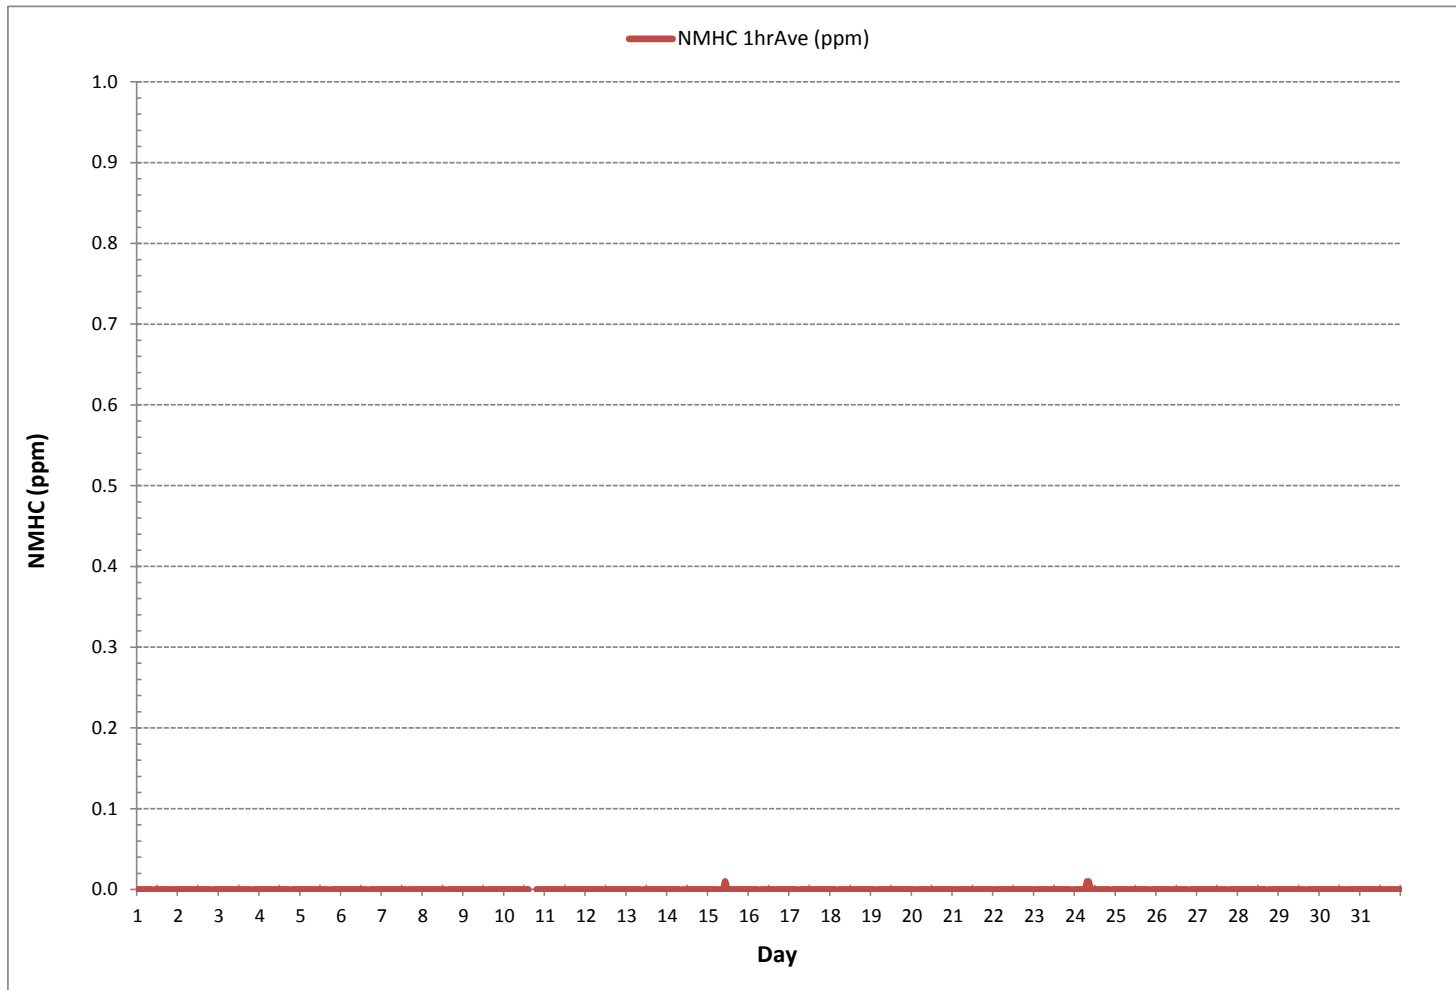

Wind: PRAMP\_986  
 Poll.: PRAMP\_986-NMHC [ppm]  
 Monthly: 18/10  
 Type: PollutionRose  
 Direction: Blowing From (Wind Frequency)  
 Based On 1 Hr.


Calm: 8.91%

Calm Avg: 0.00 [ppm]

Direction	0-0.1	0.1-0.3	0.3-1	1-2	>2.0	Total
N	6.9	0.0	0.0	0.0	0.0	6.9
NE	3.3	0.0	0.0	0.0	0.0	3.3
E	12.5	0.0	0.0	0.0	0.0	12.5
SE	18.5	0.0	0.0	0.0	0.0	18.5
S	17.8	0.0	0.0	0.0	0.0	17.8
SW	15.7	0.0	0.0	0.0	0.0	15.7
W	9.8	0.0	0.0	0.0	0.0	9.8
NW	6.7	0.0	0.0	0.0	0.0	6.7
Summary	91.1	0.0	0.0	0.0	0.0	91.1

% Icon Classes (ppm) 91 0-0.1 0 0.1-0.3 0 0.3-1 0 1-2 0 >2.0

PRAMP\_986 Poll.: PRAMP\_986-NMHC[ppm] 2018/10/01 00:00 - 2018/10/31 23:00 Calm: 8.91% Calm Poll Avg: 0.00[ppm]

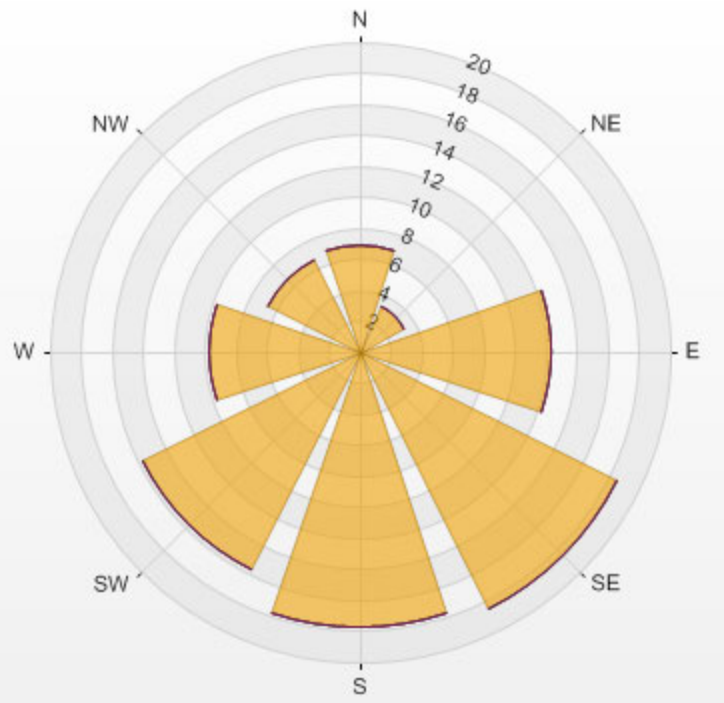

NMHC[ppm] Calibration: PRAMP\_986 Monthly: 18/10 Type: Span



■ Span Meas    — Span Ref    — Span Low    — Span High

## ***WIND SPEED***



PEACE RIVER AREA MONITORING PROGRAM COMMITTEE

Three Creeks 986b Station - October 2018

WIND SPEED Hourly Averages (WS kph)

HR START (MST)	0:00	1:00	2:00	3:00	4:00	5:00	6:00	7:00	8:00	9:00	10:00	11:00	12:00	13:00	14:00	15:00	16:00	17:00	18:00	19:00	20:00	21:00	22:00	23:00	DAILY	DAILY	24-HR	RDGS.	
HR END (MST)	0:59	1:59	2:59	3:59	4:59	5:59	6:59	7:59	8:59	9:59	10:59	11:59	12:59	13:59	14:59	15:59	16:59	17:59	18:59	19:59	20:59	21:59	22:59	23:59	MIN.	MAX.	AVG.		
DAY																													
1	1.6	1.5	1.0	1.6	1.1	2.1	1.5	0.3	2.6	5.8	8.0	8.1	8.1	8.7	7.6	8.6	9.0	7.6	8.4	7.4	7.7	6.7	4.7	3.1	0.3	0.3	9.0	4.2	24
2	1.2	1.3	1.2	2.0	1.1	2.0	1.7	2.6	4.7	5.5	11.3	13.0	9.6	9.7	11.1	11.3	9.9	6.2	4.9	7.4	7.0	6.7	4.2	1.6	1.1	1.1	13.0	5.0	24
3	1.4	1.1	1.3	2.0	1.3	0.9	0.6	1.2	0.2	0.7	0.4	2.5	2.2	1.7	5.5	2.7	1.3	2.1	2.6	3.4	3.6	5.6	5.8	6.4	0.2	6.4	0.6		24
4	5.7	4.8	5.5	5.5	5.8	5.5	4.7	4.6	5.4	7.4	5.7	3.8	4.2	5.7	5.4	8.0	6.6	5.4	4.7	5.4	6.9	4.7	5.8	5.6	3.8	8.0	1.0		24
5	5.3	4.6	5.8	6.9	5.8	6.0	5.7	5.0	4.9	4.5	5.3	4.6	4.7	5.0	3.8	3.4	8.7	4.6	2.5	3.1	6.6	9.5	9.4	8.8	2.5	9.5	2.8		24
6	7.8	7.3	8.0	7.1	4.4	4.9	4.2	5.3	4.2	3.7	3.9	5.7	5.2	5.4	10.5	10.4	10.7	6.3	4.4	5.5	3.6	4.6	5.9	5.3	3.6	10.7	3.5		24
7	6.7	5.4	7.8	6.6	7.1	6.9	7.2	6.2	7.0	7.2	7.8	8.7	9.1	9.3	9.1	8.8	9.5	8.7	8.2	7.7	7.6	6.0	6.1	6.6	5.4	9.5	7.3		24
8	5.6	6.6	8.5	5.8	7.2	6.6	8.6	10.2	10.5	10.2	12.7	9.9	7.9	7.4	8.3	11.4	9.3	6.9	4.5	5.7	6.3	5.4	4.8	5.3	4.5	12.7	7.6		24
9	2.7	0.9	4.0	7.5	5.8	8.1	6.5	6.8	6.1	5.5	11.2	9.1	8.3	6.3	7.4	8.4	9.6	6.9	6.4	6.1	6.2	7.9	10.1	7.6	0.9	11.2	6.7		24
10	9.1	9.2	10.8	9.9	10.9	11.5	8.7	10.3	8.0	4.6	7.2	8.4	7.1	4.5	4.0	3.6	3.2	2.4	2.0	2.3	2.7	3.7	3.1	3.4	2.0	11.5	5.0		24
11	4.8	4.5	2.9	3.9	5.8	9.1	8.3	10.9	14.1	15.4	17.3	13.4	11.4	11.7	10.6	9.2	6.4	5.3	5.1	5.8	3.9	3.5	2.8	2.4	2.4	17.3	7.2		24
12	2.2	0.9	2.1	4.5	4.6	5.7	6.3	5.8	7.7	9.2	8.6	8.9	9.9	9.4	9.5	11.4	7.0	7.0	6.8	4.0	2.3	1.7	0.9	0.2	0.2	11.4	5.1		24
13	0.8	0.8	1.0	0.7	1.1	0.6	0.7	0.6	1.7	4.9	3.0	4.2	5.5	6.0	5.3	5.8	6.0	6.6	7.4	4.9	5.4	6.0	5.7	4.9	0.6	7.4	2.4		24
14	4.8	5.2	4.0	7.5	8.9	9.8	9.9	9.1	9.6	9.3	9.8	9.5	10.0	10.1	10.6	10.8	7.5	7.2	7.2	5.4	7.2	5.5	4.1	4.0	4.0	10.8	7.1		24
15	9.8	8.0	3.0	2.0	4.6	5.5	3.8	3.0	3.8	2.8	2.1	4.6	8.6	9.9	11.5	7.2	4.9	4.2	2.9	0.9	0.5	0.7	1.7	2.3	0.5	11.5	2.6		24
16	2.5	2.6	2.7	2.4	3.6	3.5	3.5	4.7	3.6	5.7	5.9	7.6	6.6	7.5	9.6	10.0	6.8	5.8	4.8	6.2	7.2	6.4	6.6	8.4	2.4	10.0	4.5		24
17	7.8	7.8	8.2	9.3	9.8	6.5	9.2	11.5	13.0	11.0	10.0	8.4	8.8	12.1	10.2	11.0	9.6	6.7	5.0	5.1	10.2	11.9	9.1	7.3	5.0	13.0	8.3		24
18	3.5	2.5	1.1	2.7	1.2	3.7	4.5	11.1	10.0	11.0	4.7	7.8	9.6	15.1	18.7	19.0	19.8	10.2	7.8	8.6	2.9	1.3	1.0	0.7	0.7	19.8	6.7		24
19	2.0	1.1	2.5	3.3	3.6	2.3	2.3	2.0	1.7	1.0	2.1	4.8	7.2	7.0	10.1	13.7	12.4	8.7	7.0	11.2	14.0	8.2	10.3	12.1	1.0	14.0	5.8		24
20	11.5	11.7	11.4	8.2	11.0	9.1	6.0	6.1	7.8	12.4	15.7	16.4	22.1	16.9	20.5	15.5	12.3	11.7	9.9	10.6	11.5	10.9	7.6	7.6	6.0	22.1	10.6		24
21	6.7	5.8	6.1	4.5	3.3	3.9	2.9	3.0	2.2	1.9	10.7	11.2	8.1	9.1	10.6	10.4	5.1	3.7	5.7	6.1	4.7	4.6	5.4	5.2	1.9	11.2	3.1		24
22	5.5	4.8	5.4	7.4	7.0	7.9	7.3	5.3	8.2	11.1	15.1	11.5	10.6	11.3	10.1	8.9	4.6	1.8	2.4	1.2	3.7	5.6	9.5	6.1	1.2	15.1	6.3		24
23	5.9	6.7	3.8	5.9	6.4	1.6	1.9	3.0	3.0	6.9	7.4	4.5	3.9	3.7	4.4	0.9	2.4	1.0	1.5	2.9	2.5	2.1	2.8	4.4	0.9	7.4	2.3		24
24	2.9	3.1	2.2	3.2	3.2	1.8	2.7	3.3	3.6	2.2	4.1	6.0	5.9	5.5	6.5	5.4	5.5	5.9	5.1	3.6	3.6	4.4	4.1	4.7	1.8	6.5	3.1		24
25	3.9	3.2	3.7	4.4	5.3	3.2	6.5	6.1	4.7	6.1	6.7	7.5	9.0	9.4	9.2	9.5	8.2	8.7	12.1	12.0	10.4	9.2	7.8	8.0	3.2	12.1	6.1		24
26	8.0	8.0	6.6	6.1	5.2	4.7	7.2	5.1	4.7	5.4	5.8	8.3	6.6	8.9	10.4	6.4	5.9	4.3	6.4	4.1	5.4	8.9	8.3	10.6	4.1	10.6	6.2		24
27	7.8	6.1	6.8	8.3	10.2	12.1	6.1	7.2	8.7	9.3	13.3	14.1	14.1	11.5	21.3	11.0	3.3	0.9	2.4	1.9	2.5	2.8	2.2	3.4	0.9	21.3	5.8		24
28	4.0	4.1	4.8	5.3	2.3	1.4	1.9	3.2	3.5	5.0	5.3	5.2	4.9	5.9	4.9	5.1	4.1	3.0	2.2	1.0	0.6	2.1	3.1	1.4	0.6	5.9	2.9		24
29	2.6	2.7	1.2	2.3	2.4	2.1	2.1	2.2	4.5	5.2	6.1	5.0	6.0	6.3	7.9	6.9	5.5	3.7	3.5	3.7	3.8	3.8	4.4	3.6	1.2	7.9	3.5		24
30	2.8	3.1	3.2	2.1	3.2	2.5	2.1	1.6	2.6	2.4	5.2	5.8	5.0	4.7	6.6	7.3	3.6	3.3	4.7	3.5	3.4	4.2	6.0	6.2	1.6	7.3	3.4		24
31	4.9	4.5	4.9	4.8	4.6	4.7	4.6	3.4	3.5	3.4	5.5	6.7	6.2	4.5	4.0	1.2	3.5	5.0	6.5	7.5	8.2	7.6	8.5	7.8	1.2	8.5	0.9		24
HOURLY MAX	11.5	11.7	11.4	9.9	11.0	12.1	9.9	11.5	14.1	15.4	17.3	16.4	22.1	16.9	21.3	19.0	19.8	11.7	12.1	12.0	14.0	11.9	10.3	12.1					

STATUS FLAG CODES


C	- MONTHLY CALIBRATION	Q	- QUALITY ASSURANCE
C1	- REPEAT CALIBRATION	R	- RECOVERY
Y	- MAINTENANCE	X	- MACHINE MALFUNCTION
S	- DAILY ZERO/SPAN CHECK	G	- OUT FOR REPAIR
S1	- REPEAT ZERO/SPAN CHECK	P	- POWER FAILURE

LAST CALIBRATION:	April 4, 2018
DECLINATION :	MAGNETIC DECLINATION 15 DEGREE EAST


MONTHLY SUMMARY

NUMBER OF NON-ZERO READINGS:	744
MINIMUM 1-HR AVERAGE	0.2 kph @ HOUR 8 ON DAY 3
MAXIMUM 1-HR AVERAGE:	22.1 kph @ HOUR 12 ON DAY 20
MAXIMUM 24-HR AVERAGE:	10.6 kph ON DAY 20
MONTHLY CALIBRATION TIME:	0 hrs
OPERATIONAL TIME:	744 hrs
AMSD OPERATION UPTIME:	100.0 %
STANDARD DEVIATION:	3.4
MONTHLY AVERAGE:	1.9 kph

24 HR AVERAGES October 2018

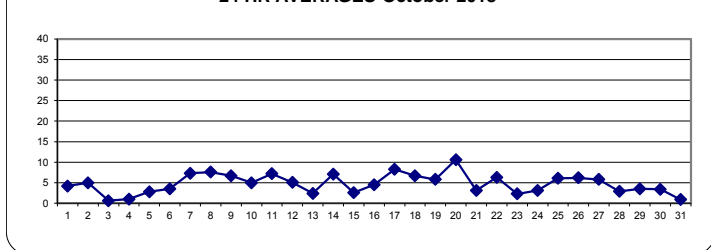

WIND SPEED Hourly Averages (WS kph)

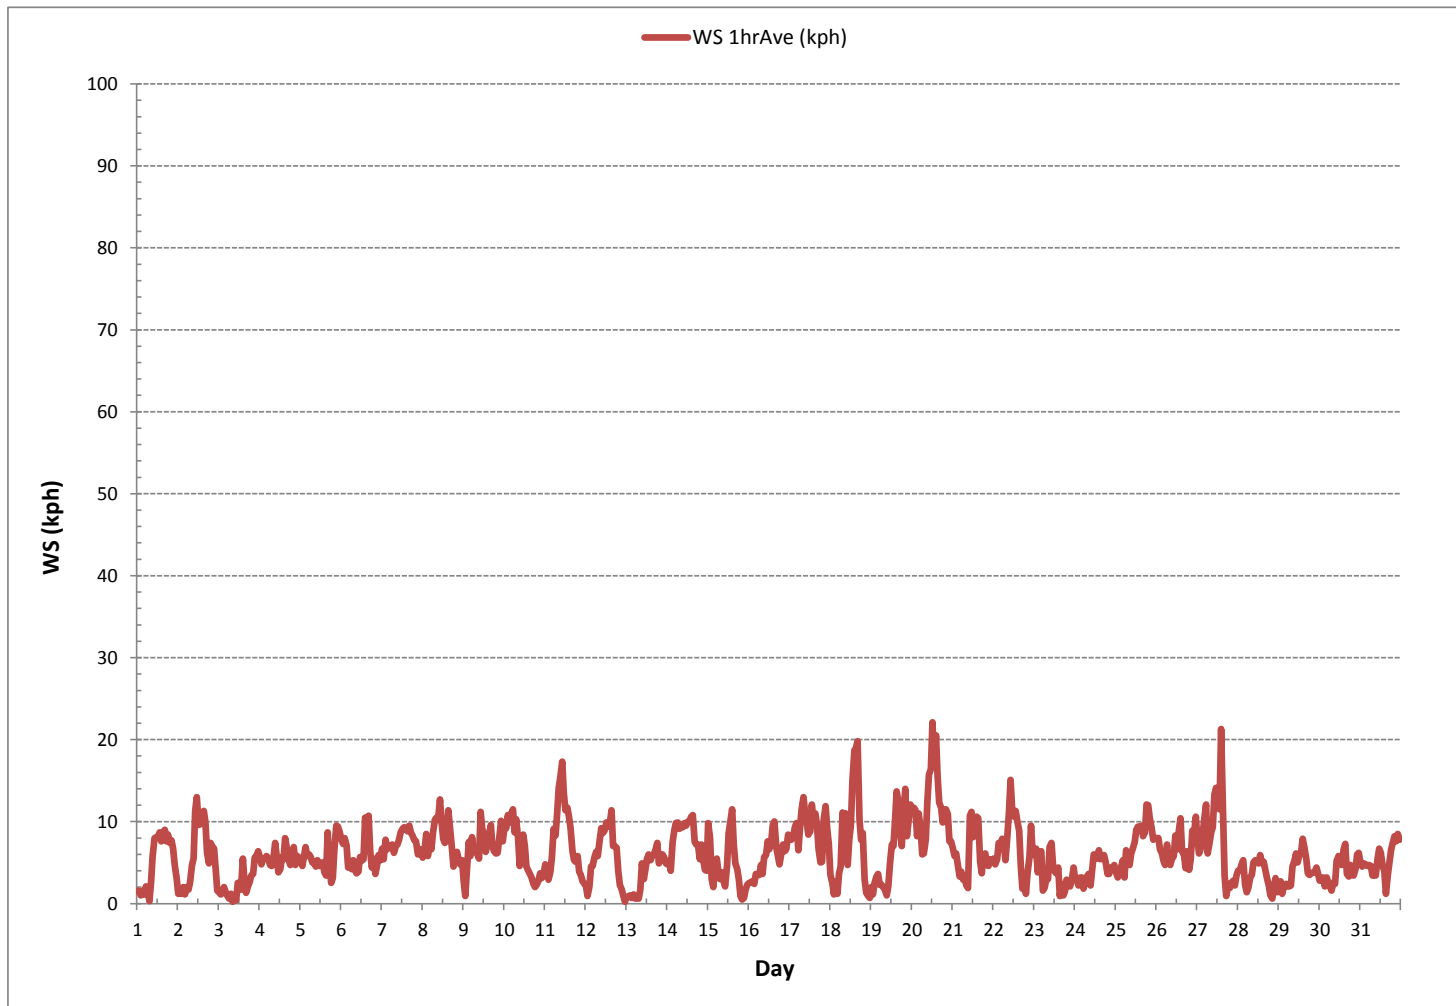

Wind: PRAMP\_986  
 Monitor: WSP [kph]  
 Monthly: 18/10  
 Type: WindRose  
 Direction: Blowing From (Wind Frequency)  
 Based On 1 Hr.

Calm: 8.60%

Direction	1.8-6.0	6.0-12.0	12.0-20.0	20.0-29.0	29.0-39.0	>39.0	Total
<b>N</b>	3.8	3.1	0.0	0.0	0.0	0.0	6.9
<b>NE</b>	1.5	1.8	0.0	0.0	0.0	0.0	3.2
<b>E</b>	9.0	3.2	0.0	0.0	0.0	0.0	12.2
<b>SE</b>	9.7	8.2	0.5	0.0	0.0	0.0	18.4
<b>S</b>	9.1	7.9	0.9	0.0	0.0	0.0	18.0
<b>SW</b>	7.3	8.2	0.3	0.0	0.0	0.0	15.7
<b>W</b>	3.4	4.6	1.8	0.3	0.0	0.0	10.0
<b>NW</b>	2.6	3.9	0.4	0.1	0.0	0.0	7.0
<b>Summary</b>	46.2	40.9	3.9	0.4	0.0	0.0	91.4



% Icon Classes (kph)

46



1.8-6.0

41



6.0-12.0

4



12.0-20.0

0



20.0-29.0

0




29.0-39.0

0



>39.0

PRAMP\_986 2018/10/01 00:00 - 2018/10/31 23:00 Calm: 8.60% Calm Wind Avg Speed: 1.09(kph)

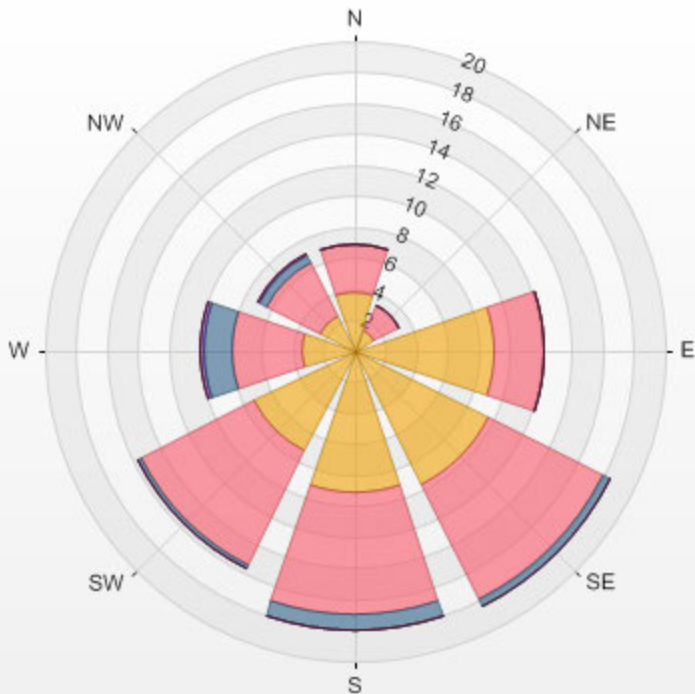

***WIND DIRECTION***



PEACE RIVER AREA MONITORING PROGRAM COMMITTEE  
Three Creeks 986b Station - October 2018

WIND DIRECTION Hourly Averages (WD)

HR START (MST)	0:00	1:00	2:00	3:00	4:00	5:00	6:00	7:00	8:00	9:00	10:00	11:00	12:00	13:00	14:00	15:00	16:00	17:00	18:00	19:00	20:00	21:00	22:00	23:00	24-HOUR AVG	24-HR		
HR END (MST)	0:59	1:59	2:59	3:59	4:59	5:59	6:59	7:59	8:59	9:59	10:59	11:59	12:59	13:59	14:59	15:59	16:59	17:59	18:59	19:59	20:59	21:59	22:59	23:59	QUADRANT	RDGS.		
DAY 1	ESE	ESE	ESE	SE	SE	SSE	SSE	SSW	WNW	NNW	NNW	NNW	NNW	N	N	NNW	NNW	N	NNW	NNW	NNW	NNW	NNW	NNW	NNW	NNW	24	
2	NW	WNW	SE	SE	S	SSE	S	WSW	W	W	WNW	WNW	WSW	W	W	W	W	SW	SW	SW	SW	SW	SW	SW	SW	W	24	
3	SW	W	W	NNW	NNW	NNE	S	SSE	NE	S	NNW	WNW	WNW	WSW	WNW	NNE	ESE	ESE	E	E	ESE	ESE	ESE	ESE	E	E	24	
4	ESE	ESE	ESE	ESE	ESE	ESE	ESE	ESE	ESE	SE	S	S	SSE	W	WNW	WNW	NNW	NNW	NNW	NNW	N	NNW	NNW	NNW	NNW	NE	24	
5	NNW	NNW	NNW	NNW	N	N	N	N	N	N	NNE	N	NNW	NNW	NW	WNW	NW	NW	NNW	E	ESE	SE	SE	ESE	N	N	24	
6	ESE	ESE	ESE	ESE	E	ENE	ENE	NE	E	NNE	NNE	N	N	NNW	NW	NW	NNW	NNE	ENE	E	ENE	ENE	ENE	ENE	NE	NE	24	
7	ENE	E	E	E	E	E	ENE	ENE	ENE	ENE	ENE	ENE	ENE	ENE	ENE	ENE	ENE	NE	NE	NE	NE	NE	ENE	E	E	ENE	24	
8	E	ESE	ESE	E	E	E	ESE	ESE	ESE	ESE	SE	ESE	ESE	ESE	ESE	SE	SE	ESE	ESE	ESE	ESE	ESE	ESE	ESE	E	ESE	24	
9	SE	NNW	SE	SE	SE	SE	SE	ESE	ESE	E	SE	SE	SE	ESE	SE	SE	ESE	ESE	ESE	ESE	ESE	SE	SE	ESE	SE	ESE	24	
10	SE	SE	SE	SE	SE	SE	SE	SE	SE	SE	SE	SSE	S	SSW	SSW	W	W	W	W	SSW	SSW	S	SSW	SSW	SSE	SSW	24	
11	SSW	SSW	SSW	SSW	SSE	SSE	SSE	SSE	SSE	SSE	S	SSW	SSW	SSW	SSW	SW	SW	SW	SW	SW	SW	SW	SSW	S	SSW	S	24	
12	S	S	N	N	N	N	N	NNW	NNW	NNW	NNW	NNW	NNW	NW	NW	NW	NW	NW	NW	NNW	W	WSW	W	ENE	NNW	NNW	24	
13	W	SW	SE	SSE	SE	SSE	SW	WSW	WNW	WNW	NW	NNW	WNW	WSW	WSW	SW	SSW	S	SSE	SSE	S	SSW	SSW	S	SW	SW	24	
14	SSE	S	SE	S	SSW	S	S	S	SSW	SSW	SSW	SSW	SSW	SW	SW	SW	SW	WSW	WSW	WSW	WSW	SW	SW	WNW	SSW	SSW	24	
15	WNW	WNW	WSW	S	SSE	S	SSW	SW	SW	WSW	W	NW	WNW	WNW	NW	NNW	NNW	N	W	SSE	SSW	SE	SE	W	W	W	24	
16	ESE	ESE	ESE	ESE	ESE	ESE	SE	SE	SSE	SSE	S	S	S	SSW	SW	SW	SSW	S	S	SW	SW	SW	SW	SW	S	SW	24	
17	SSW	SSW	SSW	SSW	S	SSW	SSW	SSW	SSW	SSW	SSW	SSW	SSW	SW	WSW	WSW	WSW	WSW	SW	SW	SW	W	W	WSW	WSW	SW	24	
18	WSW	SSW	S	WSW	WSW	SSW	WSW	WNW	WNW	NW	NW	W	W	W	WNW	NW	NNW	NW	NW	WNW	WNW	WNW	WNW	ENE	WNW	WNW	24	
19	SSE	ESE	ESE	ESE	SE	ESE	ESE	E	ESE	SSW	NE	E	SE	S	SSE	SSE	SSE	SE	ESE	SE	SE	ESE	SE	SSE	SE	SE	24	
20	S	S	S	SSW	SW	SW	SW	SW	SW	WSW	WSW	W	W	W	W	W	WSW	W	SSW	WSW	WSW	WSW	WSW	WSW	WSW	WSW	24	
21	WSW	SW	SW	SSW	S	SSE	SSW	SW	W	W	WNW	WNW	WNW	W	WNW	WNW	WSW	S	SSE	SSE	SE	ESE	ESE	ESE	WSW	WSW	24	
22	ESE	ESE	ESE	SE	SE	SE	SE	ESE	SE	SSE	S	S	S	S	S	S	SSW	S	E	E	ESE	ESE	SE	SE	SSE	SE	24	
23	ESE	SE	ESE	SE	SE	E	E	ESE	ESE	SSE	S	SSE	S	WNW	WNW	W	WNW	WNW	SE	ESE	ESE	ESE	E	ESE	SE	SE	24	
24	ESE	E	E	ESE	E	ESE	E	ESE	ESE	ESE	SW	S	SSE	SW	S	SSW	SSW	SSE	S	SSE	S	S	SE	SE	SSE	SE	24	
25	ESE	ESE	SE	ESE	SE	ESE	SE	SE	SE	SSW	S	S	S	S	SSW	SSW	S	SSE	S	SSW	SSW	SSW	SSW	SSW	SSW	S	SSW	24
26	SW	SSW	SSW	SSW	SSW	SSE	SSW	SSW	SE	ESE	S	SSW	SSW	S	SSW	S	SSE	S	S	SSW	SE	S	S	SSW	S	SSW	24	
27	SSW	SSW	SSW	SW	WSW	W	WSW	WSW	WSW	W	WNW	WNW	WNW	W	WNW	WNW	NW	SSE	S	ESE	ESE	ESE	SE	ESE	W	W	24	
28	ESE	ESE	ESE	ESE	E	NE	ENE	ESE	E	ESE	E	E	E	NE	ENE	E	E	E	ENE	NNE	NNE	ESE	SW	W	E	E	24	
29	SW	SW	W	SSW	SSW	S	ESE	S	S	SSW	SSW	S	SSW	SSW	SSW	SSW	S	SSE	SSW	SSW	SSW	SSW	SE	SE	ESE	S	24	
30	ESE	SSE	SE	SE	SE	SSE	SE	SE	SSE	SSW	SSW	SSW	SSW	SSW	SSW	SSW	SSW	SSW	SSW	SSW	SSW	SSW	SSW	SSW	SSW	SSW	SSW	24
31	SSW	SSW	SE	SE	SE	SE	SE	SE	SE	S	SSW	SW	WSW	WSW	WNW	N	NNW	NNW	NNW	NNW	NNW	NNW	NNW	NNW	NNW	WNW	24	


STATUS FLAG CODES

C	- MONTHLY CALIBRATION	Q	- QUALITY ASSURANCE
C1	- REPEAT CALIBRATION	R	- RECOVERY
Y	- MAINTENANCE	X	- MACHINE MALFUNCTION
S	- DAILY ZERO/SPAN CHECK	G	- OUT FOR REPAIR
S1	- REPEAT ZERO/SPAN CHECK	P	- POWER FAILURE

LAST CALIBRATION:	April 4, 2018
DECLINATION :	MAGNETIC DECLINATION 15 DEGREE EAST

MONTHLY CALIBRATION TIME:	0 hrs	OPERATIONAL TIME:	744 hrs
STANDARD DEVIATION:	82	AMD OPERATION UPTIME:	100.0 %
		MONTHLY AVERAGE:	194 (SSW)

**WIND DIRECTION Hourly Averages (WD)**

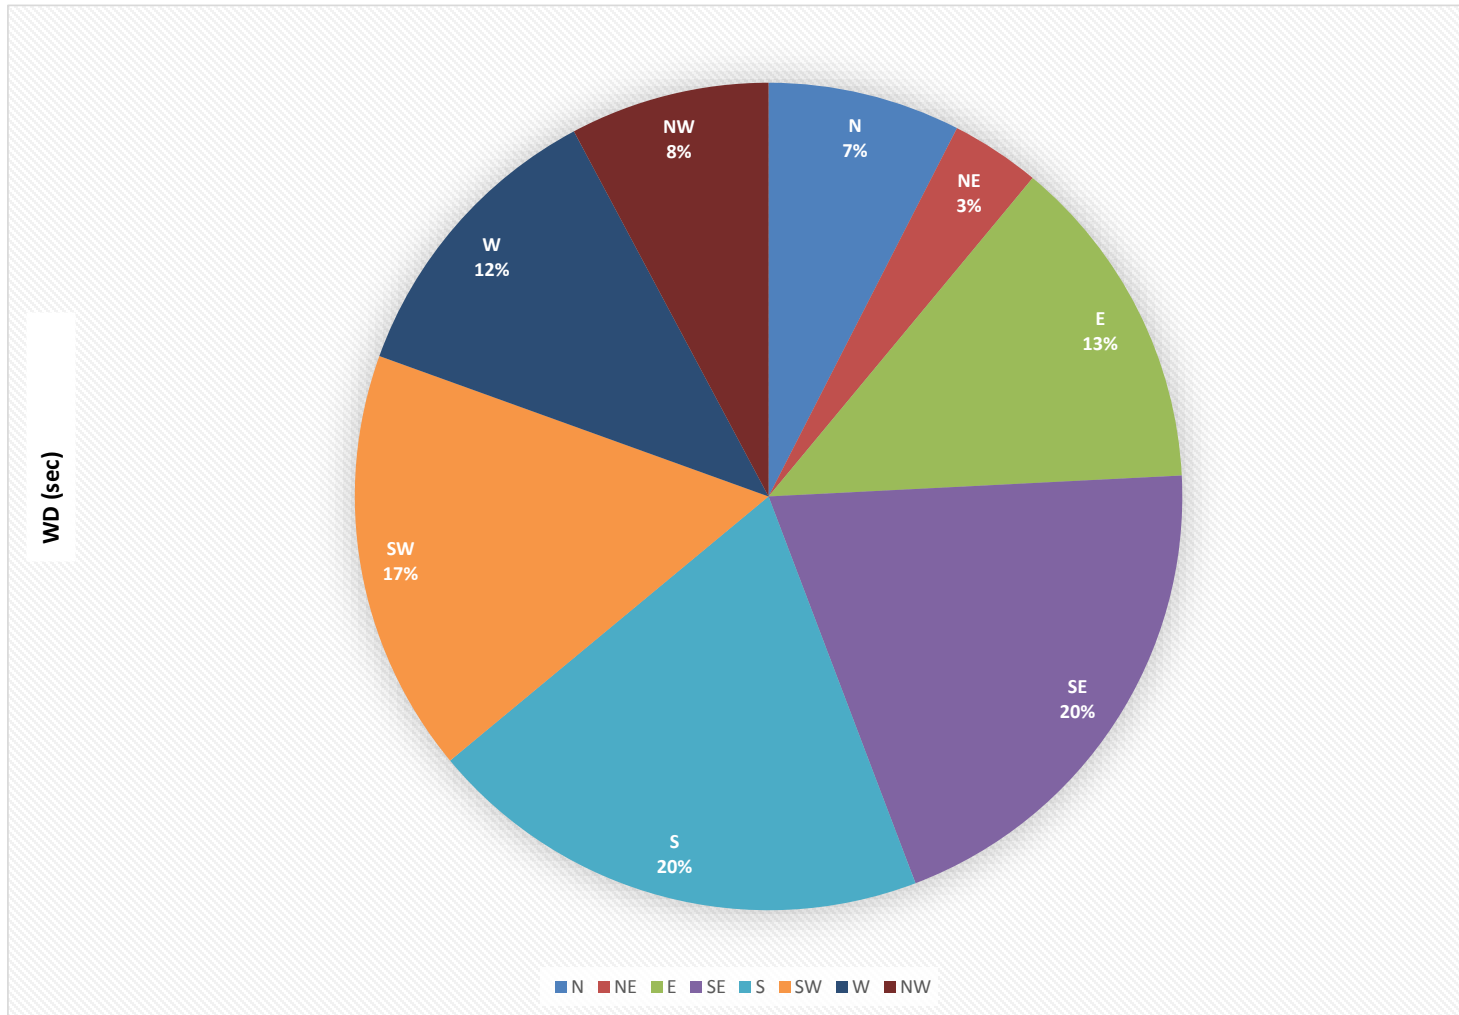

WDR[degwdr] Station: PRAMP\_986 Monthly: 18/10 Type: AVG 1 Hr. [1 Hr.]



— WDR[degwdr]

***RELATIVE HUMIDITY***



RELATIVE HUMIDITY Hourly Averages (RH %)

HR START (MST)	0:00	1:00	2:00	3:00	4:00	5:00	6:00	7:00	8:00	9:00	10:00	11:00	12:00	13:00	14:00	15:00	16:00	17:00	18:00	19:00	20:00	21:00	22:00	23:00	DAILY	DAILY	24-HR	RDGS.	
HR END (MST)	0:59	1:59	2:59	3:59	4:59	5:59	6:59	7:59	8:59	9:59	10:59	11:59	12:59	13:59	14:59	15:59	16:59	17:59	18:59	19:59	20:59	21:59	22:59	23:59	MIN.	MAX.	AVG.		
DAY																													
1	83	81	83	83	80	80	77	75	72	67	71	75	81	68	64	66	70	73	65	64	64	66	69	74	64	83	73	24	
2	80	85	87	88	85	85	83	78	76	71	55	48	45	39	35	33	34	38	43	46	49	52	54	60	33	88	60	24	
3	64	67	68	68	73	81	85	87	84	68	54	51	48	44	43	42	41	43	55	61	66	64	62	64	41	87	62	24	
4	64	66	67	69	70	71	71	71	68	59	51	49	45	40	39	37	40	44	53	58	58	65	69	76	37	76	58	24	
5	83	84	83	85	85	86	84	81	78	76	71	64	61	59	59	55	58	63	71	72	74	75	75	76	55	86	73	24	
6	77	77	79	79	80	80	80	81	81	76	69	63	57	54	58	63	69	73	85	88	91	88	85	86	54	91	76	24	
7	86	86	86	86	85	86	86	88	89	86	84	85	81	78	77	75	72	70	68	69	71	72	73	73	68	89	80	24	
8	75	76	76	76	75	75	76	73	75	78	78	74	66	59	53	52	52	55	65	72	75	79	81	82	52	82	71	24	
9	85	89	87	84	84	83	83	83	82	80	77	69	61	53	51	50	51	58	65	69	73	76	77	78	50	89	73	24	
10	79	80	80	80	80	79	77	76	76	75	74	73	72	72	74	77	78	79	80	81	82	82	80	80	72	82	78	24	
11	80	80	80	81	82	82	80	77	75	73	70	65	61	58	55	57	59	62	65	68	71	76	81	83	55	83	72	24	
12	89	95	98	96	96	98	99	99	99	97	96	96	95	92	87	84	81	78	79	82	84	86	85	88	78	99	91	24	
13	89	90	92	93	93	94	95	94	92	87	72	63	64	65	64	64	67	75	85	91	91	91	89	88	63	95	83	24	
14	90	87	91	87	85	85	85	82	81	77	74	71	62	56	48	46	48	42	42	44	43	44	46	53	42	91	65	24	
15	51	51	55	63	64	65	67	65	60	59	58	56	57	55	54	53	55	62	70	80	82	84	85	88	51	88	64	24	
16	89	91	91	92	95	95	93	87	80	69	60	52	40	30	26	25	26	32	38	31	33	34	36	37	25	95	58	24	
17	39	40	42	41	41	37	37	39	33	32	29	26	23	21	22	23	25	23	25	27	28	24	23	26	30	21	42	30	24
18	33	36	41	42	46	51	52	52	53	48	45	43	39	34	32	28	29	32	37	39	48	60	64	65	28	65	44	24	
19	69	71	78	79	78	83	86	88	81	67	55	48	43	40	36	34	34	40	49	47	46	49	49	47	34	88	58	24	
20	43	45	48	51	53	59	64	66	62	49	41	36	31	31	28	29	29	34	37	38	41	42	44	46	28	66	44	24	
21	49	51	52	57	59	60	58	61	56	47	38	36	34	33	32	31	32	38	47	50	52	56	58	63	31	63	48	24	
22	62	63	62	59	58	57	60	66	61	48	39	35	32	29	27	25	26	37	51	61	66	64	58	61	25	66	50	24	
23	72	72	77	75	70	79	85	87	82	66	54	47	40	38	36	34	38	52	66	76	79	81	83	83	34	87	66	24	
24	85	85	87	89	89	90	90	90	89	78	73	66	55	47	47	44	46	54	58	63	62	64	73	77	44	90	71	24	
25	80	83	85	87	84	87	85	86	86	71	66	61	58	53	44	45	47	55	56	54	57	60	61	59	44	87	67	24	
26	60	68	72	75	77	79	79	74	75	67	59	55	56	52	50	53	54	59	62	73	90	77	73	71	50	90	67	24	
27	69	69	67	64	65	69	72	63	63	66	66	60	55	53	46	46	49	60	73	77	76	79	82	84	46	84	66	24	
28	83	81	84	80	82	85	87	87	84	78	75	72	69	67	67	67	70	74	78	81	85	87	84	84	67	87	79	24	
29	87	93	95	96	95	96	97	98	96	92	85	77	72	72	75	76	78	85	86	84	82	90	97	100	72	100	88	24	
30	100	100	100	100	100	100	100	100	100	95	85	83	82	76	62	58	62	69	74	72	67	68	69	70	58	100	83	24	
31	73	76	86	90	92	95	96	95	94	86	76	68	66	64	67	71	75	82	95	99	100	100	100	100	64	100	85	24	
HOURLY MAX	100	100	100	100	100	100	100	100	100	97	96	96	95	92	87	84	81	85	95	99	100	100	100	100					
HOURLY AVG	73	75	77	77	77	79	80	79	77	71	65	60	56	53	50	50	51	56	62	65	67	69	70	72					


STATUS FLAG CODES

C	- MONTHLY CALIBRATION	Q	- QUALITY ASSURANCE
C1	- REPEAT CALIBRATION	R	- RECOVERY
Y	- MAINTENANCE	X	- MACHINE MALFUNCTION
S	- DAILY ZERO/SPAN CHECK	G	- OUT FOR REPAIR
S1	- REPEAT ZERO/SPAN CHECK	P	- POWER FAILURE


MONTHLY SUMMARY

MINIMUM 1-HR AVERAGE:	21	%	@ HOUR	13	ON DAY	17
MAXIMUM 1-HR AVERAGE:	100	%	@ HOUR	23	ON DAY	29
MAXIMUM 24-HR AVERAGE:	91	%			ON DAY	12
OPERATIONAL TIME:						744 hrs
AMD OPERATION UPTIME:						100.0 %
STANDARD DEVIATION:	19		MONTHLY AVERAGE:			67 %

24 HR AVERAGES October 2018

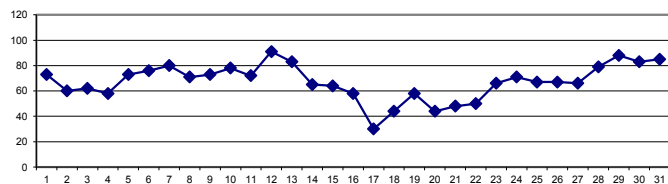

RELATIVE HUMIDITY Hourly Averages (RH %)

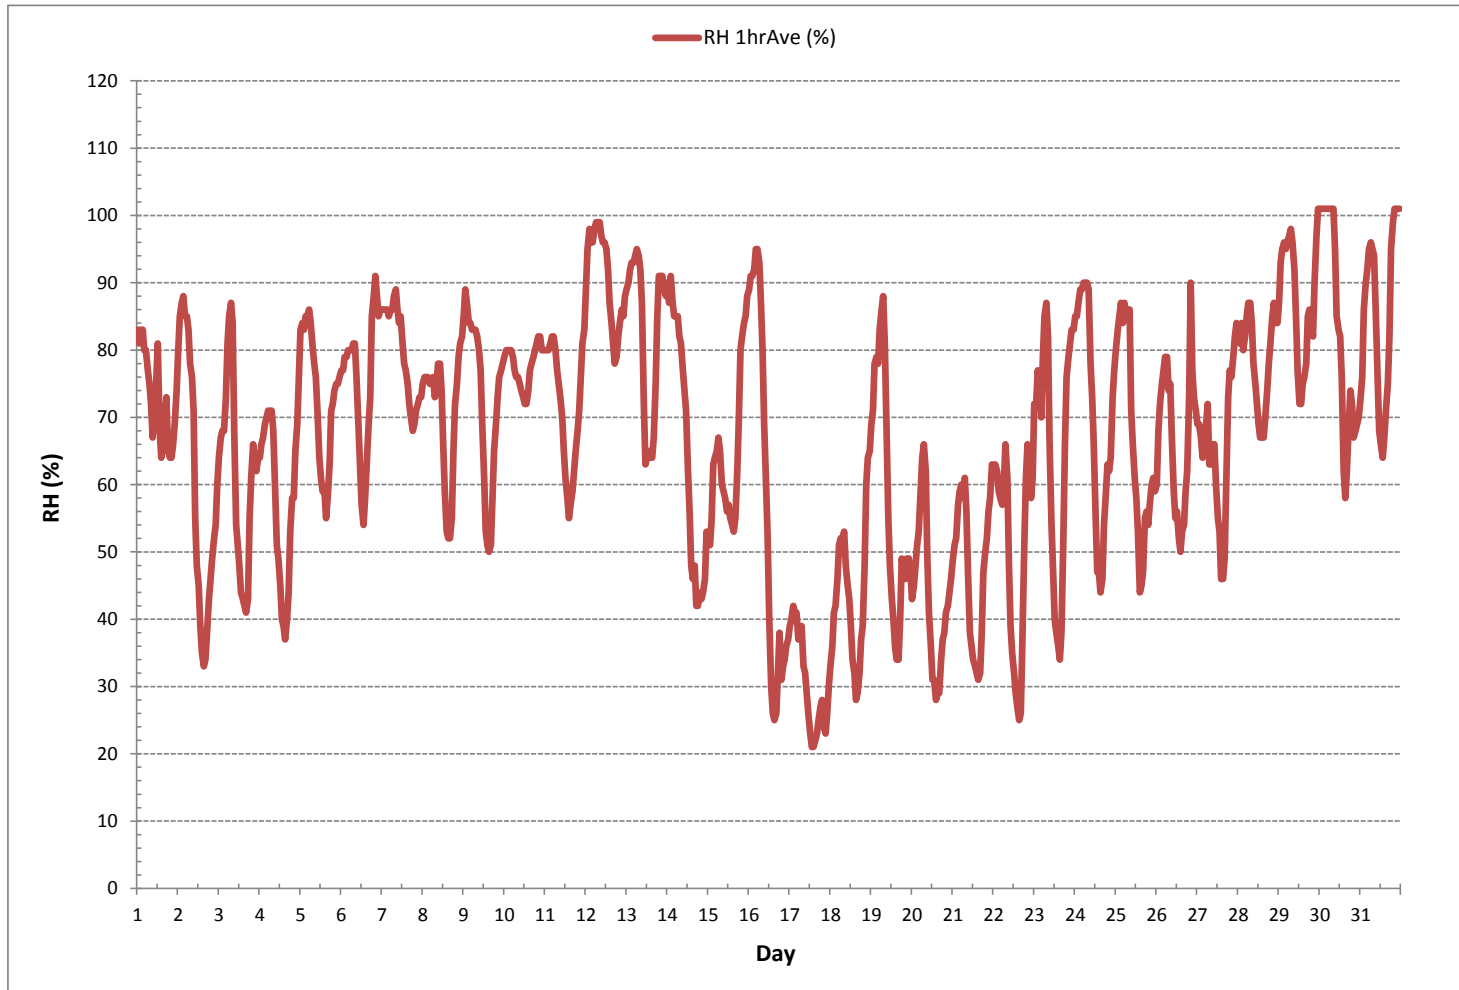



## ***BAROMETRIC PRESSURE***




BAROMETRIC PRESSURE Hourly Averages (BP mbar)

HR START (MST)	0:00	1:00	2:00	3:00	4:00	5:00	6:00	7:00	8:00	9:00	10:00	11:00	12:00	13:00	14:00	15:00	16:00	17:00	18:00	19:00	20:00	21:00	22:00	23:00	DAILY	DAILY	24-HR	RDGS.			
HR END (MST)	0:59	1:59	2:59	3:59	4:59	5:59	6:59	7:59	8:59	9:59	10:59	11:59	12:59	13:59	14:59	15:59	16:59	17:59	18:59	19:59	20:59	21:59	22:59	23:59	MIN.	MAX.	AVG.				
DAY																															
1	944	944	943	943	943	943	943	943	943	944	945	945	946	946	947	947	948	948	949	950	950	951	951	951	951	951	943	951	946	24	
2	951	951	950	950	949	949	948	948	948	947	946	945	944	943	942	942	941	941	940	940	940	940	940	940	940	940	940	940	951	945	24
3	940	941	941	942	942	943	943	944	944	945	945	945	945	945	945	944	944	944	944	943	943	943	943	943	943	940	945	943	24		
4	942	942	942	941	941	940	940	940	940	940	940	939	939	939	939	939	940	940	940	941	941	942	942	942	942	939	942	940	24		
5	942	943	943	943	943	943	944	944	944	944	944	944	944	944	944	944	943	943	943	943	942	942	942	942	941	941	944	943	24		
6	941	940	940	940	940	940	940	941	941	942	942	943	943	944	945	945	946	947	947	948	948	948	949	949	949	940	949	944	24		
7	949	949	949	949	950	950	950	950	950	951	951	951	951	952	952	953	953	953	953	954	954	954	955	955	955	949	955	952	24		
8	955	955	955	955	955	955	955	955	955	955	955	955	954	954	953	953	953	952	952	952	952	952	953	953	952	952	955	954	24		
9	954	954	955	955	955	956	956	956	956	956	957	956	956	956	956	955	955	955	954	954	954	954	954	953	953	953	957	955	24		
10	952	952	952	951	951	950	950	950	950	950	950	950	949	949	949	949	949	949	949	949	949	948	948	947	947	947	947	952	950	24	
11	946	946	945	945	944	942	942	942	941	940	939	938	937	936	935	935	934	934	934	933	933	933	933	933	933	933	933	946	938	24	
12	932	932	932	931	931	932	932	933	935	936	938	939	941	942	943	944	945	946	947	947	948	948	949	949	949	949	949	949	940	24	
13	949	950	950	950	950	951	951	951	952	952	952	953	953	953	953	952	952	951	951	951	951	950	950	949	949	949	949	953	951	24	
14	949	948	948	947	946	945	944	944	943	943	942	942	942	941	941	940	940	940	940	940	940	941	941	942	942	940	949	943	24		
15	942	943	943	943	943	944	944	944	944	945	945	945	945	946	946	947	947	948	948	948	948	949	949	949	949	942	949	946	24		
16	949	949	949	949	948	948	948	948	948	948	948	948	948	947	947	946	946	945	945	945	944	944	944	944	944	944	949	947	24		
17	944	943	943	943	942	942	941	941	940	940	940	939	939	939	938	938	938	937	937	937	937	937	937	938	938	937	944	940	24		
18	939	939	939	940	940	940	940	941	941	942	943	944	944	944	945	945	946	946	947	947	948	948	949	949	939	949	944	24			
19	950	950	951	951	951	952	952	952	953	954	954	953	953	952	952	950	949	949	947	946	944	943	942	941	941	941	954	950	24		
20	941	941	940	940	940	939	940	939	940	939	940	939	940	940	940	940	941	941	941	941	941	942	942	942	939	942	940	24			
21	943	943	944	944	945	945	946	946	947	947	948	948	948	948	948	948	948	948	948	947	948	948	947	947	943	948	947	24			
22	947	947	947	946	945	945	945	944	944	944	944	944	944	943	943	943	942	942	941	941	941	941	941	941	941	941	947	943	24		
23	941	940	940	940	940	940	940	939	939	940	939	939	939	939	939	938	938	937	937	936	936	936	936	936	936	936	941	939	24		
24	936	936	936	936	936	936	936	936	936	936	936	936	936	936	936	936	935	935	935	935	935	935	935	935	935	935	936	936	24		
25	935	935	935	935	935	935	935	935	935	935	936	936	936	936	935	935	934	934	934	934	934	935	935	935	935	934	936	935	24		
26	935	935	935	935	934	934	934	934	935	934	934	933	933	933	933	932	932	931	931	931	931	931	931	931	931	931	935	933	24		
27	931	931	931	931	931	932	933	933	934	935	936	937	938	938	939	939	939	939	940	940	940	940	940	940	931	940	936	24			
28	940	939	939	939	938	937	937	936	936	936	936	935	935	934	933	933	933	933	934	934	934	935	935	935	933	940	936	24			
29	935	935	936	936	936	936	936	936	937	937	937	937	937	938	938	938	938	938	938	938	938	938	938	938	938	935	938	937	24		
30	938	938	939	939	939	939	939	939	939	939	940	940	939	939	939	939	939	939	939	938	938	938	938	937	937	940	939	24			
31	937	937	936	936	935	935	934	934	934	934	933	933	933	933	933	934	934	935	936	937	939	940	941	933	941	935	24				
HOURLY MAX	955	955	955	955	956	956	956	956	956	957	956	956	956	956	955	955	955	954	954	954	954	955	955	955	955	955	955	955	24		
HOURLY AVG	943	943	943	943	943	943	943	943	943	943	943	943	943	943	943	943	943	943	943	943	943	943	943	943	943	943	943	943	24		

STATUS FLAG CODES

C	- MONTHLY CALIBRATION	Q	- QUALITY ASSURANCE
C1	- REPEAT CALIBRATION	R	- RECOVERY
Y	- MAINTENANCE	X	- MACHINE MALFUNCTION
S	- DAILY ZERO/SPAN CHECK	G	- OUT FOR REPAIR
S1	- REPEAT ZERO/SPAN CHECK	P	- POWER FAILURE


24 HR AVERAGES October 2018

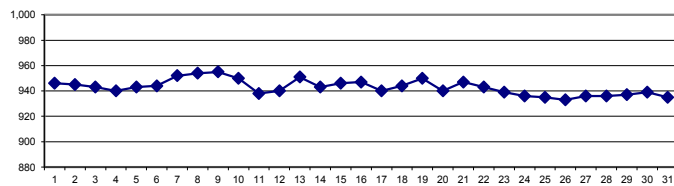

MONTHLY SUMMARY

MINIMUM 1-HR AVERAGE:	931 mbar	@ HOUR	3	ON DAY	12
MAXIMUM 1-HR AVERAGE:	957 mbar	@ HOUR	10	ON DAY	9
MAXIMUM 24-HR AVERAGE:	955 mbar			ON DAY	9
OPERATIONAL TIME:					744 hrs
AMD OPERATION UPTIME:					100.0 %
STANDARD DEVIATION:	6	MONTHLY AVERAGE:	943 mbar		

BAROMETRIC PRESSURE Hourly Averages (BP mbar)

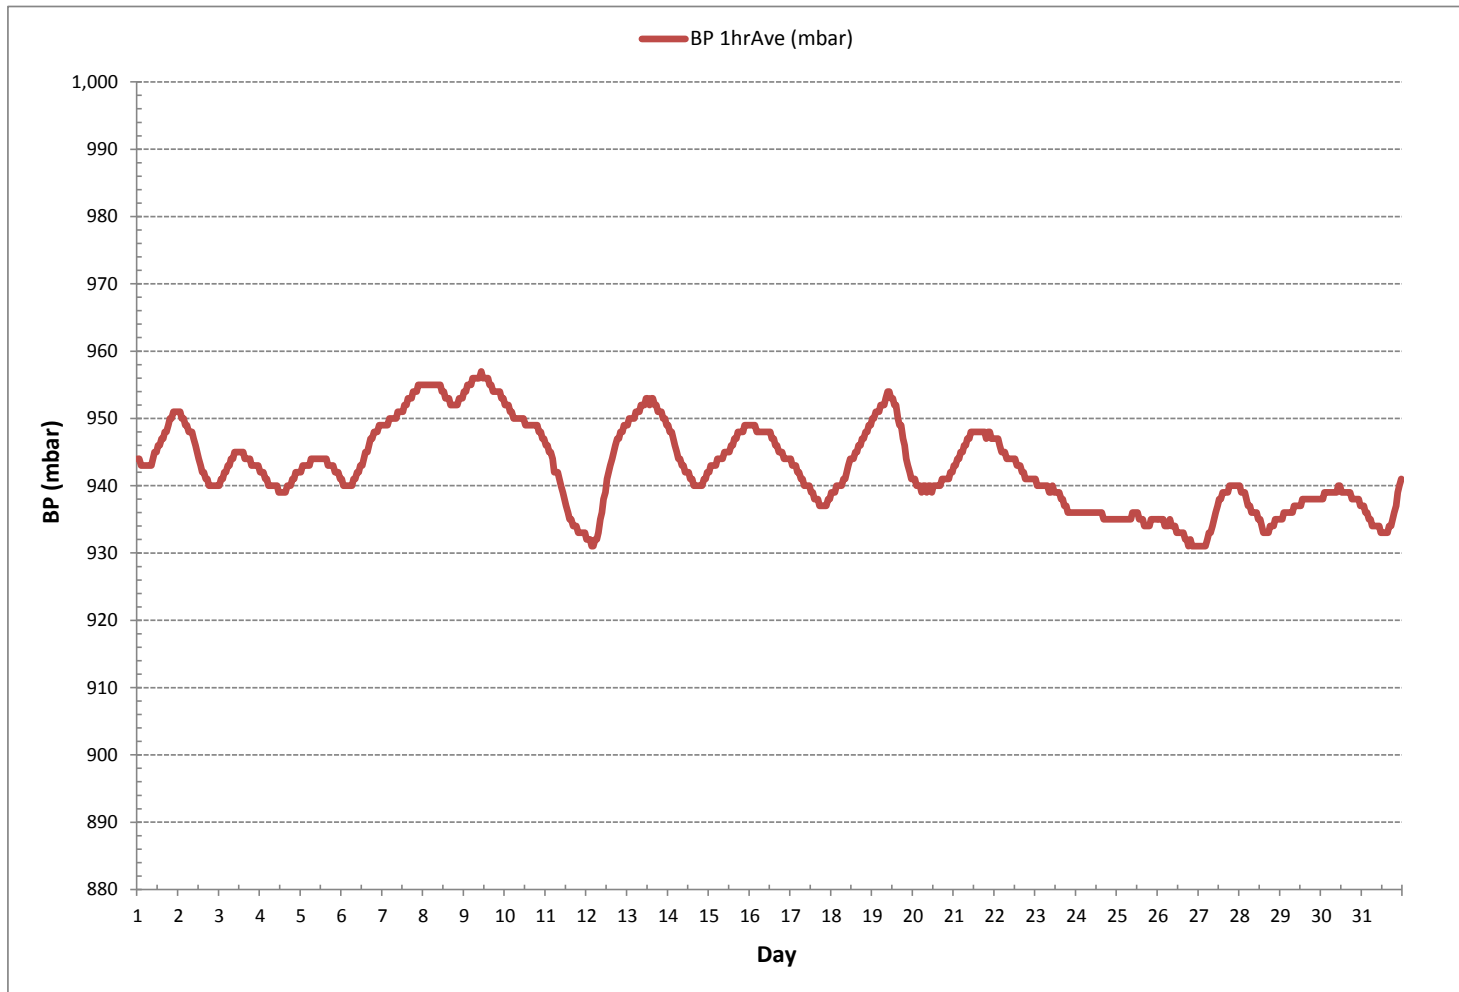

***AMBIENT TEMPERATURE***




AMBIENT TEMPERATURE Hourly Averages (AmbTPX °C)

HR START (MST)	0:00	1:00	2:00	3:00	4:00	5:00	6:00	7:00	8:00	9:00	10:00	11:00	12:00	13:00	14:00	15:00	16:00	17:00	18:00	19:00	20:00	21:00	22:00	23:00	DAILY	DAILY	24-HR	RDGS.
HR END (MST)	0:59	1:59	2:59	3:59	4:59	5:59	6:59	7:59	8:59	9:59	10:59	11:59	12:59	13:59	14:59	15:59	16:59	17:59	18:59	19:59	20:59	21:59	22:59	23:59	MIN.	MAX.	AVG.	
DAY																												
1	-4.7	-3.7	-3.9	-3.5	-3.4	-3.5	-3.0	-2.7	-1.7	-0.1	1.1	1.3	0.9	1.7	1.5	0.8	0.2	-0.6	-0.8	-1.2	-1.6	-2.0	-2.7	-4.4	-4.7	1.7	-1.5	24
2	-6.1	-7.6	-8.7	<b>-8.8</b>	-6.6	-7.2	-6.6	-5.0	-3.6	-2.3	-0.4	0.7	1.8	2.7	3.4	3.9	4.0	3.4	2.0	1.5	0.9	0.6	-0.1	-1.5	<b>-8.8</b>	4.0	-1.6	24
3	-2.2	-2.5	-2.3	-2.3	-3.5	-5.7	-7.8	-7.9	-5.3	-1.0	0.8	1.2	2.1	3.2	3.4	3.9	4.2	3.4	-0.3	-1.9	-2.8	-2.8	-2.5	-2.7	-7.9	4.2	-1.3	24
4	-2.6	-2.9	-3.1	-3.2	-2.9	-2.3	-2.0	-1.7	-0.7	1.6	3.9	4.8	6.4	6.9	7.3	7.7	7.4	4.8	2.0	1.4	0.1	-2.0	-2.8	-3.2	-3.2	7.7	1.0	24
5	-4.1	-3.9	-3.4	-3.3	-3.2	-3.1	-3.1	-3.1	-3.0	-2.6	-1.9	-0.6	0.0	0.4	0.4	1.6	1.0	-0.6	-2.2	-2.1	-2.0	-1.9	-2.2	-2.4	-4.1	1.6	-1.9	24
6	-2.3	-2.1	-2.1	-1.7	-1.7	-2.0	-2.2	-2.4	-1.9	-0.4	1.3	2.8	4.1	5.0	4.0	3.6	2.4	1.8	0.6	-0.5	-1.3	-1.5	-1.7	-1.9	-2.4	5.0	0.0	24
7	-2.1	-2.1	-2.3	-2.5	-2.7	-2.8	-2.8	-2.9	-2.8	-2.3	-1.9	-1.8	-1.1	-0.9	-0.9	-1.0	-0.8	-0.9	-1.0	-1.3	-1.6	-1.8	-2.0	-2.6	-2.9	-0.8	-1.9	24
8	-3.1	-3.1	-3.3	-3.3	-3.2	-3.7	-4.1	-4.1	-4.1	-3.7	-3.5	-2.9	-1.5	0.2	1.5	1.7	1.7	0.7	-1.8	-3.1	-3.4	-3.9	-4.3	-4.8	-4.8	1.7	-2.5	24
9	-5.3	-6.5	-4.4	-3.6	-3.6	-3.7	-3.7	-3.8	-3.7	-3.5	-2.8	-1.0	0.6	2.4	2.9	3.2	2.8	1.1	-0.9	-2.3	-3.2	-2.9	-2.2	-2.1	-6.5	3.2	-1.9	24
10	-2.1	-2.3	-2.4	-2.4	-2.3	-2.2	-2.0	-1.9	-1.7	-1.3	-1.0	-0.6	-0.3	0.0	0.1	-0.1	-0.3	-0.4	-0.6	-0.8	-0.9	-1.1	-1.1	-1.1	-2.4	0.1	-1.2	24
11	-1.2	-1.2	-1.3	-1.6	-2.2	-2.9	-2.7	-2.2	-1.5	-0.2	1.0	2.5	3.7	4.4	4.9	5.2	5.3	5.3	5.0	5.1	5.1	4.8	4.5	4.6	-2.9	5.3	1.8	24
12	4.0	3.5	2.9	2.4	1.1	0.5	0.2	-0.3	-0.7	-1.1	-0.9	-0.8	-0.9	-1.0	-0.4	-0.2	-0.4	-0.9	-1.1	-1.2	-1.4	-1.4	-1.4	-1.6	-1.6	4.0	-0.1	24
13	-1.6	-1.5	-1.7	-1.7	-1.5	-1.6	-1.6	-1.3	-0.8	0.0	1.9	2.9	3.0	3.5	4.6	5.5	5.6	3.8	1.9	0.8	1.3	1.7	1.8	0.8	-1.7	5.6	1.1	24
14	-0.2	0.7	-1.0	0.2	0.3	0.0	0.0	0.7	1.5	3.0	4.8	6.5	8.8	9.9	10.8	11.2	10.6	11.0	10.3	9.3	10.0	9.9	9.4	8.1	-1.0	11.2	5.7	24
15	9.1	9.1	7.8	6.0	5.8	5.8	5.8	6.4	8.1	8.8	9.8	10.9	12.0	12.4	12.9	13.2	13.0	11.6	10.0	8.1	7.2	6.7	6.9	6.0	5.8	13.2	8.9	24
16	5.3	4.5	4.3	3.8	2.3	2.0	0.3	0.8	2.2	5.5	7.5	9.7	12.8	15.3	16.3	16.9	16.6	14.1	11.2	13.0	12.3	12.0	10.8	10.9	0.3	16.9	8.8	24
17	10.2	10.0	9.3	10.1	10.4	11.5	11.1	9.9	11.3	12.2	14.6	16.6	18.3	<b>19.3</b>	19.1	18.6	18.1	16.9	15.8	15.2	16.4	16.3	15.1	13.9	9.3	<b>19.3</b>	<b>14.2</b>	24
18	12.9	12.0	10.5	10.1	9.2	7.4	7.6	8.1	8.1	9.6	11.2	12.1	13.4	14.0	13.8	13.9	13.1	11.2	8.9	8.2	4.9	1.6	0.8	0.2	0.2	14.0	9.3	24
19	-0.8	-1.1	-2.4	-2.5	-2.0	-3.2	-4.1	-4.7	-2.1	3.7	6.3	8.8	10.8	12.9	13.4	13.5	12.9	10.1	6.6	7.8	8.1	7.9	7.7	8.7	-4.7	13.5	4.8	24
20	11.0	10.9	10.3	9.8	10.0	8.7	7.8	8.2	8.8	11.0	13.7	14.2	14.5	14.2	14.9	14.5	14.2	12.6	12.2	11.3	10.3	9.8	8.6	7.8	7.8	14.9	11.2	24
21	7.1	6.3	5.4	3.5	2.3	1.7	1.8	0.8	2.5	6.6	8.5	9.5	10.7	11.9	13.1	13.0	12.1	8.4	5.0	4.5	3.5	2.1	1.3	0.2	0.2	13.1	5.9	24
22	0.1	0.0	0.4	1.0	1.5	1.5	0.8	-0.9	1.0	6.2	9.1	11.0	12.1	13.7	14.6	15.5	14.7	10.5	4.3	1.4	0.2	1.5	4.6	3.9	-0.9	15.5	5.4	24
23	0.6	1.0	-0.4	0.2	1.6	-1.5	-3.6	-4.2	-1.2	5.1	8.7	10.9	13.4	14.5	14.8	15.6	14.1	9.7	4.0	0.5	-0.8	-1.1	-2.3	-1.5	-4.2	15.6	4.1	24
24	-2.6	-2.6	-3.6	-4.2	-4.4	-4.6	-5.0	-5.0	-4.3	0.6	5.7	8.2	10.3	12.3	12.7	13.4	12.6	9.9	8.5	6.9	7.3	6.7	3.2	2.1	-5.0	13.4	3.5	24
25	1.8	0.8	0.4	0.1	1.2	0.3	1.4	1.0	1.1	6.7	8.5	9.5	10.1	12.1	14.2	14.3	13.2	10.8	10.4	10.8	10.6	10.0	9.2	8.7	0.1	14.3	7.0	24
26	7.8	5.8	4.4	3.4	2.6	1.5	0.9	1.7	1.0	3.5	6.7	7.2	7.3	8.0	8.3	7.6	6.7	5.1	4.6	5.8	4.8	5.3	5.6	6.2	0.9	8.3	5.1	24
27	6.3	6.2	6.7	7.1	7.5	7.3	6.8	6.9	6.5	6.4	6.7	7.2	8.4	9.4	11.0	10.6	9.2	6.0	1.4	0.1	0.0	-1.2	-2.7	-3.3	-3.3	11.0	5.4	24
28	-2.9	-2.7	-3.5	-2.1	-2.5	-3.2	-3.7	-3.5	-1.9	0.1	1.9	3.5	4.3	4.7	4.5	4.4	3.7	3.0	2.5	1.5	0.8	0.4	0.9	0.5	-3.7	4.7	0.4	24
29	0.5	0.7	1.0	1.3	1.0	0.2	-1.0	-1.4	-1.3	-0.6	1.5	3.2	4.9	5.3	5.8	6.1	5.8	3.3	2.3	2.1	2.8	-0.9	-2.4	-2.2	-2.4	6.1	1.6	24
30	-2.6	-3.7	-1.4	-0.6	-0.5	-1.0	-1.8	-2.3	-1.2	1.6	4.3	4.8	5.2	6.8	8.7	8.7	7.2	5.3	3.9	4.7	5.5	4.8	4.8	4.2	-3.7	8.7	2.7	24
31	3.8	3.2	0.9	0.1	-0.2	-1.2	-1.1	-0.6	-0.6	2.0	4.0	5.6	6.2	6.5	6.1	5.1	3.6	0.7	-1.7	-2.0	-2.0	-1.9	-2.2	-2.4	-2.4	6.5	1.3	24
HOURLY MAX	12.9	12.0	10.5	10.1	10.4	11.5	11.1	9.9	11.3	12.2	14.6	16.6	18.3	19.3	19.1	18.6	18.1	16.9	15.8	15.2	16.4	16.3	15.1	13.9				
HOURLY AVG	1.1	0.8	0.4	0.4	0.3	-0.2	-0.6	-0.6	0.3	2.4	4.2	5.4	6.5	7.5	8.0	8.1	7.6	5.8	4.0	3.3	2.9	2.4	2.0	1.6				

STATUS FLAG CODES

C	- MONTHLY CALIBRATION	Q	- QUALITY ASSURANCE
C1	- REPEAT CALIBRATION	R	- RECOVERY
Y	- MAINTENANCE	X	- MACHINE MALFUNCTION
S	- DAILY ZERO/SPAN CHECK	G	- OUT FOR REPAIR
S1	- REPEAT ZERO/SPAN CHECK	P	- POWER FAILURE


24 HR AVERAGES October 2018

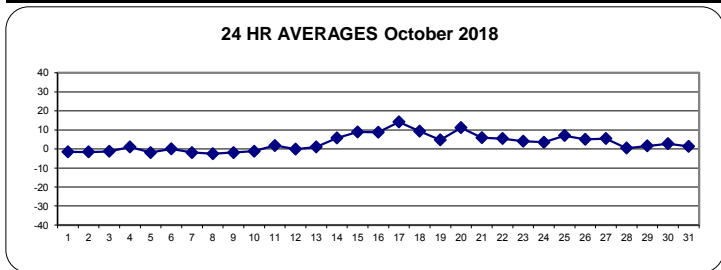

MONTHLY SUMMARY

MINIMUM 1-HR AVERAGE:	-8.8 °C	@ HOUR	3	ON DAY	2
MAXIMUM 1-HR AVERAGE:	19.3 °C	@ HOUR	13	ON DAY	17
MAXIMUM 24-HR AVERAGE:	14.2 °C			ON DAY	17
OPERATIONAL TIME:				744	hrs
AMD OPERATION UPTIME:				100.0	%
STANDARD DEVIATION:	5.7			MONTHLY AVERAGE:	3.1 °C

AMBIENT TEMPERATURE Hourly Averages (AmbTPX °C)

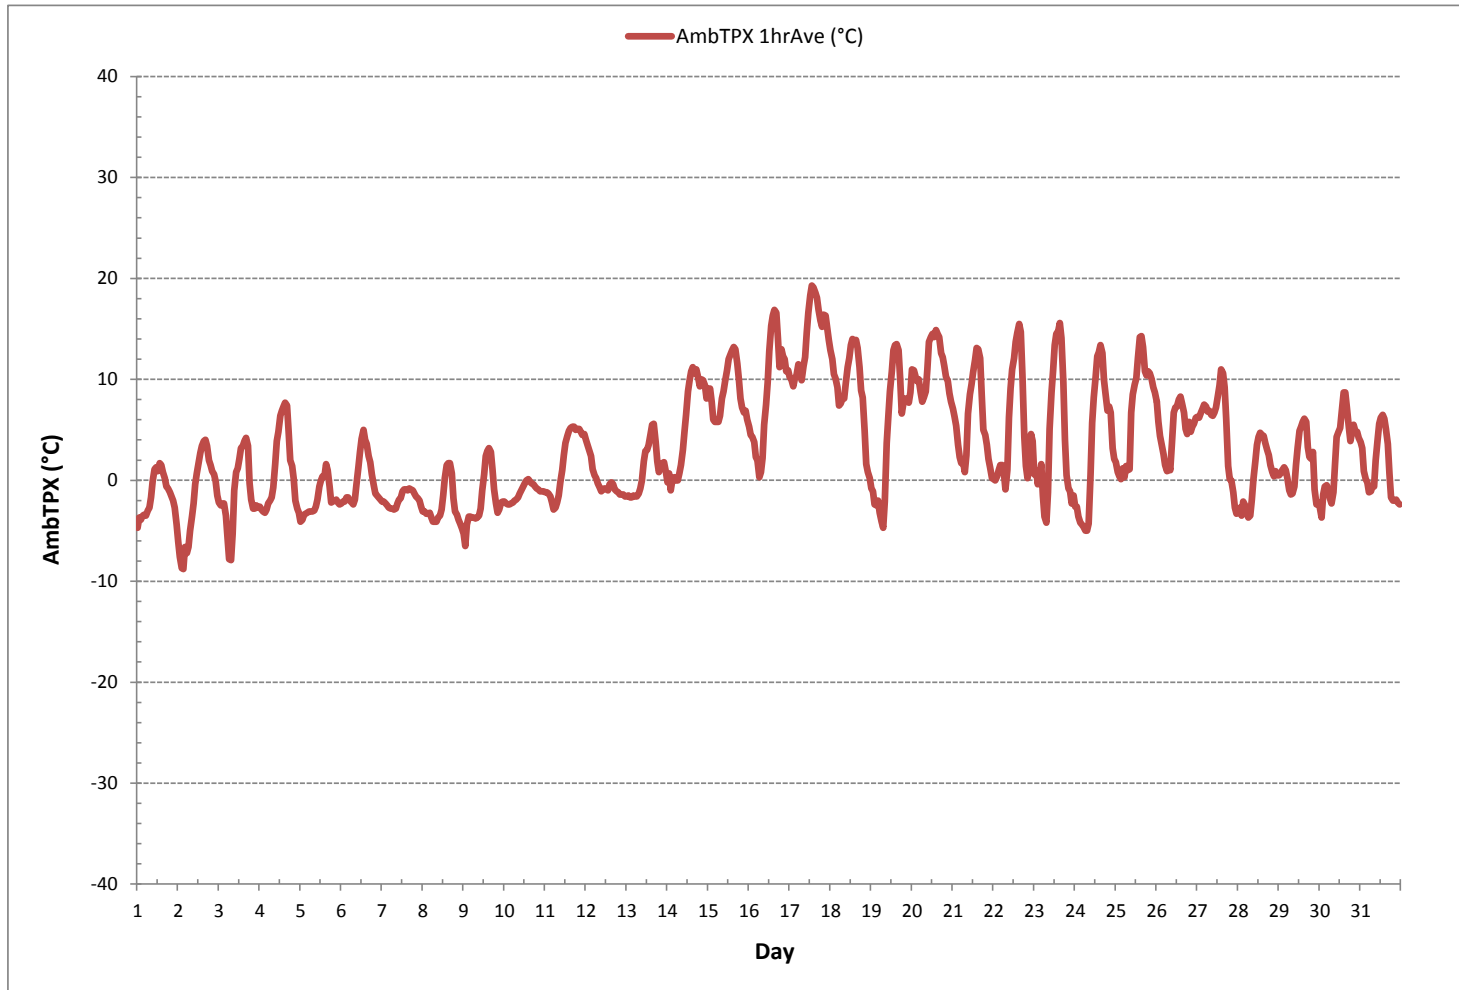

***STATION TEMPERATURE***




STATION TEMPERATURE Hourly Averages (StnTPX °C)

HR START (MST)	0:00	1:00	2:00	3:00	4:00	5:00	6:00	7:00	8:00	9:00	10:00	11:00	12:00	13:00	14:00	15:00	16:00	17:00	18:00	19:00	20:00	21:00	22:00	23:00	DAILY	DAILY	24-HR	RDGS.	
HR END (MST)	0:59	1:59	2:59	3:59	4:59	5:59	6:59	7:59	8:59	9:59	10:59	11:59	12:59	13:59	14:59	15:59	16:59	17:59	18:59	19:59	20:59	21:59	22:59	23:59	MIN.	MAX.	AVG.		
DAY																													
1	24.1	24.2	23.9	23.8	24.0	24.0	23.9	23.8	23.8	23.6	23.6	23.2	22.9	22.5	22.3	23.4	23.4	23.6	23.7	23.9	24.0	23.9	24.0	24.2	22.3	24.2	23.7	24	
2	24.3	24.3	24.3	24.0	24.2	24.0	24.2	24.0	24.0	23.8	23.9	24.2	22.7	20.8	20.4	20.0	19.3	19.9	22.9	23.4	23.6	23.7	23.8	24.2	19.3	24.3	23.1	24	
3	24.1	24.3	24.0	23.9	24.2	24.1	24.2	24.2	24.2	24.2	24.3	23.5	21.9	21.4	21.6	21.1	20.6	19.9	22.7	23.7	24.1	23.8	24.0	23.7	19.9	24.3	23.2	24	
4	23.7	23.9	23.8	23.9	23.6	23.5	23.5	23.4	23.3	23.1	23.2	22.7	22.0	22.5	22.3	21.9	21.6	21.5	23.5	23.9	23.7	23.8	24.0	24.2	21.5	24.2	23.2	24	
5	24.2	24.3	24.1	23.9	23.7	23.7	23.9	23.8	23.7	23.6	23.2	22.9	22.7	21.7	22.2	20.9	19.6	20.9	23.4	23.7	23.4	22.4	22.4	22.7	19.6	24.3	23.0	24	
6	22.8	22.7	22.7	22.7	23.4	23.3	23.4	23.2	23.2	23.4	23.4	23.2	22.1	22.0	21.7	22.6	23.0	23.3	23.4	23.2	23.4	23.4	23.2	23.3	21.7	23.4	23.0	24	
7	23.1	23.1	23.0	23.0	22.9	23.0	23.0	23.1	23.0	22.8	22.7	22.5	22.4	22.4	22.6	22.6	22.6	22.8	22.8	23.1	23.0	23.0	23.2	22.9	22.4	23.2	22.9	24	
8	23.2	22.9	22.6	23.0	22.8	22.8	22.3	22.1	21.9	21.9	21.3	21.8	21.8	20.9	19.8	19.5	19.6	20.2	23.1	23.8	23.7	23.8	23.7	23.7	19.5	23.8	22.2	24	
9	23.9	24.1	23.9	22.8	23.2	22.8	22.8	23.1	22.7	23.0	21.9	22.1	21.3	20.7	20.0	19.3	19.2	21.7	23.1	23.7	23.7	23.3	22.3	22.5	19.2	24.1	22.4	24	
10	22.4	22.4	21.9	22.1	21.9	21.8	22.3	22.1	22.4	23.1	22.8	22.6	23.1	23.3	23.4	22.4	22.2	23.4	23.8	23.7	23.6	23.6	23.7	23.8	21.8	23.8	22.8	24	
11	23.7	23.7	23.8	23.6	23.6	23.2	23.3	23.0	22.4	21.7	21.0	21.7	22.1	21.8	21.9	22.3	22.8	22.8	23.1	23.1	23.1	23.0	23.1	23.1	21.0	23.8	22.8	24	
12	23.0	23.0	23.0	23.1	23.3	23.1	23.2	23.2	23.3	23.1	23.3	23.1	23.3	23.2	23.3	23.2	23.4	23.4	23.5	23.6	23.6	23.5	23.5	23.5	23.0	23.6	23.3	24	
13	23.4	23.6	23.5	23.5	23.4	23.5	23.4	23.5	23.5	23.4	23.7	23.6	21.9	21.5	20.6	20.3	20.9	22.9	23.3	23.5	23.6	23.5	23.5	23.5	20.3	23.7	22.8	24	
14	23.6	23.4	23.6	23.5	23.2	23.1	22.9	22.9	23.1	23.0	22.9	22.6	22.0	21.7	21.5	21.9	22.1	22.7	22.7	23.1	22.9	22.6	22.8	23.1	21.5	23.6	22.8	24	
15	22.8	22.7	23.0	23.1	23.2	23.3	23.1	22.8	22.9	22.5	22.3	22.3	22.8	23.4	23.4	23.5	23.3	22.8	22.5	22.7	23.1	23.1	23.1	23.4	22.3	23.5	23.0	24	
16	23.4	23.5	23.6	23.8	23.9	24.1	24.0	23.8	22.9	23.3	22.6	22.0	22.6	23.2	23.3	23.4	22.7	22.4	22.8	23.2	23.0	23.1	23.1	23.1	22.0	24.1	23.2	24	
17	23.1	23.1	23.0	23.0	22.6	22.9	22.7	22.6	22.5	22.7	23.3	24.2	24.2	22.4	23.9	23.5	23.0	22.5	23.1	22.8	22.7	23.1	23.1	22.7	22.4	24.2	23.0	24	
18	22.2	22.7	22.8	23.1	23.2	23.4	23.6	23.4	23.6	23.5	23.5	24.1	23.6	23.0	22.9	22.7	22.6	22.4	23.4	23.4	23.7	24.0	24.0	24.1	22.2	24.1	23.3	24	
19	24.1	24.2	24.0	24.2	24.1	24.2	24.1	24.2	24.4	24.6	24.0	22.9	23.1	22.8	22.6	22.5	22.5	22.3	23.3	23.3	22.6	21.1	22.5	22.6	22.3	21.1	24.6	23.3	24
20	22.1	22.1	22.2	22.6	22.7	23.0	23.3	23.4	23.6	23.4	23.0	23.5	23.7	23.6	23.3	22.8	22.8	22.5	23.0	23.2	23.3	23.3	23.5	23.7	22.1	23.7	23.1	24	
21	23.7	23.7	23.9	23.9	23.9	23.9	24.2	24.0	24.4	24.5	23.7	23.5	23.5	22.9	22.6	22.4	22.2	22.4	23.7	23.6	23.7	24.0	24.1	24.0	22.2	24.5	23.6	24	
22	24.0	24.0	23.9	23.7	23.6	23.3	23.5	24.0	23.9	22.6	22.2	21.9	22.6	22.9	22.8	22.7	22.6	22.6	23.6	23.9	23.8	23.9	23.5	23.6	21.9	24.0	23.3	24	
23	23.7	23.9	24.1	24.2	23.9	24.0	24.0	24.2	24.4	24.1	23.0	23.4	23.4	23.2	23.2	22.6	22.2	22.7	23.7	23.9	24.1	24.1	24.1	24.0	22.2	24.4	23.7	24	
24	24.1	24.1	24.1	24.2	24.1	24.1	24.2	24.1	24.0	24.4	24.1	23.2	22.5	22.8	22.5	22.3	22.3	22.5	23.3	23.6	23.7	23.6	23.8	24.0	22.3	24.4	23.6	24	
25	24.0	24.0	24.1	24.1	24.0	24.1	23.9	23.8	24.1	23.8	22.9	22.4	21.7	21.6	22.5	22.6	22.5	22.3	22.5	22.4	22.5	22.6	22.8	23.1	21.6	24.1	23.1	24	
26	23.3	23.5	23.7	23.6	23.9	23.8	23.8	23.8	23.9	24.0	23.5	22.7	22.4	21.9	21.3	22.2	23.0	23.1	23.3	23.2	23.2	22.9	22.9	22.9	21.3	24.0	23.2	24	
27	23.0	23.2	23.2	23.2	23.1	24.0	23.4	23.3	23.3	23.2	23.4	23.2	22.8	22.6	22.5	22.0	21.9	23.4	23.8	24.0	24.1	24.2	24.2	24.2	21.9	24.2	23.3	24	
28	24.1	24.0	24.1	24.1	24.0	23.9	24.0	23.9	23.9	23.6	23.3	23.0	22.9	22.4	22.6	22.8	23.0	23.3	23.5	23.6	23.5	23.8	23.8	23.8	22.4	24.1	23.5	24	
29	23.7	23.7	23.7	23.6	23.8	23.9	24.1	24.0	23.9	23.9	23.7	23.3	22.3	21.5	21.3	20.6	21.6	23.3	23.8	23.9	23.9	24.1	24.1	24.1	20.6	24.1	23.3	24	
30	24.3	24.2	23.9	23.6	23.7	24.1	24.1	24.2	24.1	24.5	23.9	23.1	22.6	22.6	22.3	21.8	21.5	23.4	23.4	23.7	23.4	23.5	23.6	23.7	21.5	24.5	23.5	24	
31	24.1	23.6	23.7	23.9	23.9	23.9	23.9	23.9	23.7	23.8	23.6	23.2	21.9	21.8	22.6	23.2	23.3	23.7	23.8	23.9	23.9	23.8	23.8	23.8	21.8	24.1	23.5	24	
HOURLY MAX	24.3	24.3	24.3	24.2	24.2	24.2	24.2	24.2	24.4	24.6	24.3	24.2	24.2	23.6	23.9	23.5	23.4	23.7	23.8	24.0	24.1	24.2	24.2	24.2					
HOURLY AVG	23.5	23.6	23.5	23.5	23.5	23.5	23.6	23.5	23.5	23.4	23.1	23.0	22.6	22.3	22.2	22.1	22.0	22.4	23.3	23.4	23.4	23.5	23.5	23.5					

STATUS FLAG CODES

C	- MONTHLY CALIBRATION	Q	- QUALITY ASSURANCE
C1	- REPEAT CALIBRATION	R	- RECOVERY
Y	- MAINTENANCE	X	- MACHINE MALFUNCTION
S	- DAILY ZERO/SPAN CHECK	G	- OUT FOR REPAIR
S1	- REPEAT ZERO/SPAN CHECK	P	- POWER FAILURE

24 HR AVERAGES October 2018

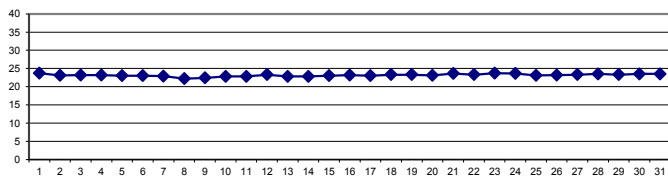


MONTHLY SUMMARY

MINIMUM 1-HR AVERAGE:	19.2 °C	@ HOUR	16	ON DAY	9
MAXIMUM 1-HR AVERAGE:	24.6 °C	@ HOUR	9	ON DAY	19
MAXIMUM 24-HR AVERAGE:	23.7 °C			ON DAY	1
OPERATIONAL TIME:					744 hrs
AMD OPERATION UPTIME:					100.0 %
STANDARD DEVIATION:	0.9				
MONTHLY AVERAGE:					23.1 °C



STATION TEMPERATURE Hourly Averages (StnTPX °C)

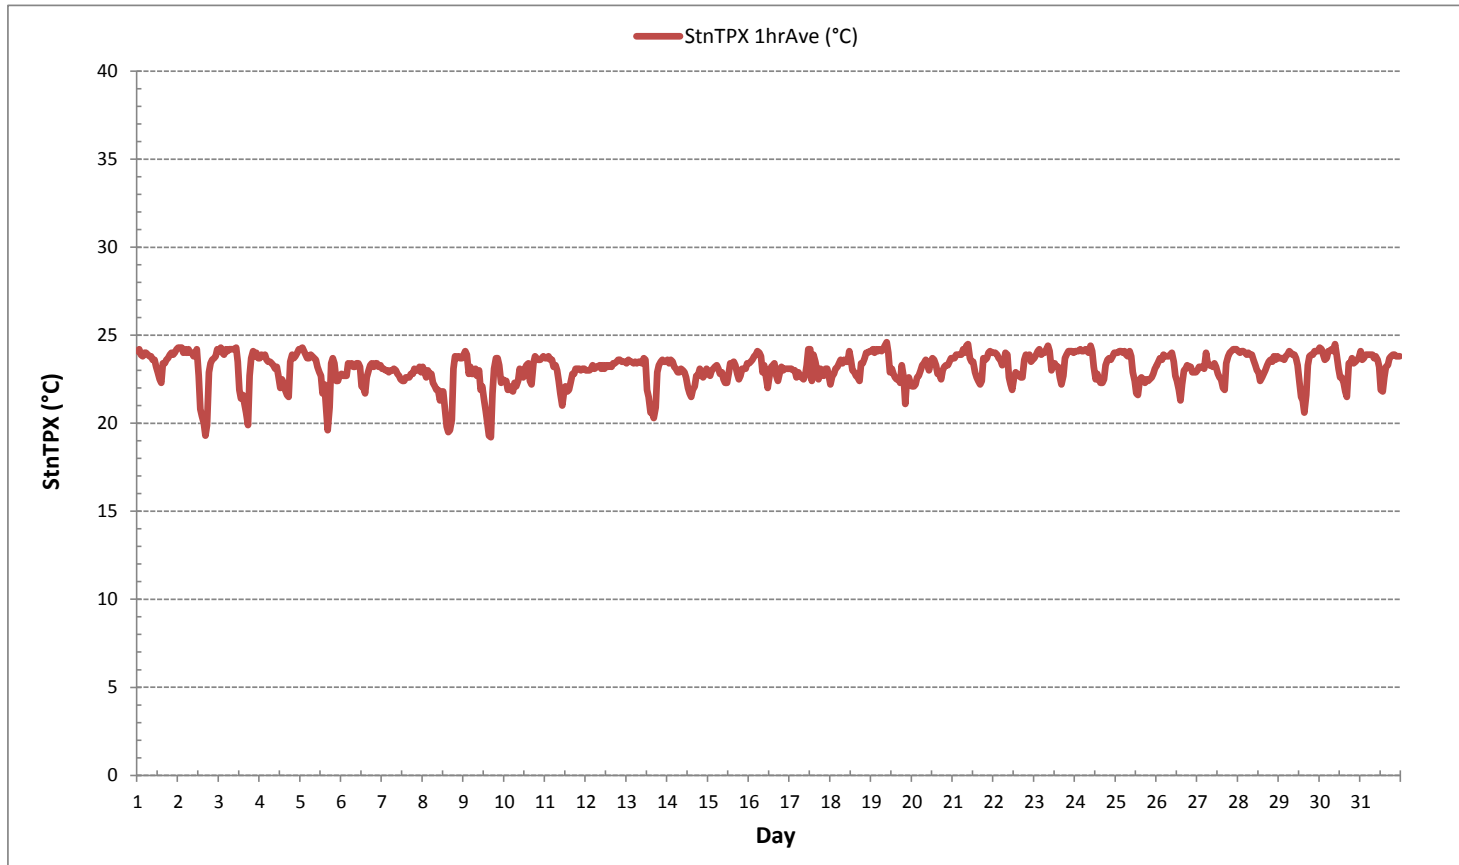

***APPENDIX II  
EQUIPMENT CALIBRATION RESULTS***

***SULPHUR DIOXIDE***



### Thermo 43C Sulphur Dioxide Analyzer Calibration

Date:	October 11, 2018	Barometer/B.P./units:	Brunton 05535 expires December 15, 2018	27.83	inHg
Company/Airshed:	PRAMP	Thermometer/Station Temp:	F.S. 160459244 expires June 19, 2020	23.2	°C
Location/Station Name:	986B	Weather Conditions:	Cloudy/Overcast		
Parameter:	Sulphur Dioxide	Calibration Purpose:	routine monthly		
Start Time 24 hr. (mst):	7:41	Performed By/Reviewer:	Limin Li	Rob Fisher	
End Time 24 hr. (mst):	10:05	Cal Gas Expiry Date:	December 8, 2019		
Calibration Method:	Gas Dilution	Converter Model & s/n (if applicable):	n/a		
Analyzer:					
Serial Number/Owner:	43C-62339-335   Maxxam	Range ppb:	500		
Last Calibration Date:	September 11, 2018	As Found C.F.:	0.980		
Previous C.F.:	0.997	New C.F.:	0.999		

Calibration Standards:		Standard Calibration Points for Ranges	
Low Flow Meter ID/Expiry Date:	n/a	Point	ppb
High Flow Meter ID/Expiry Date:	n/a	High	380
Calibrator ID/Expiry Date:	Sabio id# 17200415 expires August 21, 2019	Mid	180
Cal Gas Cylinder I.D. #:	EY0000769	Low	90
Cal Gas Conc. (ppm):	50.5		


ALL POINTS ARE 15 MINUTES OF STABILITY AS OF SEPTEMBER 23, 2015

Point	Calibrator Flow Rates (cc/min)			Calculated Concentration (ppb):	Indicated Concentration (ppb):	Correction Factors (C.F.):
	Diluent	Cal Gas	Total			
as found zero	6000	0.00	6000	0.0	-1.5	n/a
as found high	5953	45.10	5998	379.7	386	0.980
adjusted zero	6000	0.00	6000	0.0	0.0	n/a
adjusted high	5953	45.10	5998	379.7	380	0.999
mid	5978	21.40	5999	180.1	181	0.995
low	5988	10.70	5999	90.1	91.5	0.984
calibrator zero	6000	0.00	6000	0.0	0.0	n/a
Average C.F. =						0.993

Linear Regression/Calibration Results:

Correlation Coefficient =	1.000	LIMITS	> or = 0.995
Slope =	1.000		0.95-1.05
b (Intercept as % of full scale) =	-0.14%		± 3% F.S.
% change in C.F. from last cal =	1.71%		± 10%


Thermo 43C Sulphur Dioxide Analyzer Calibration

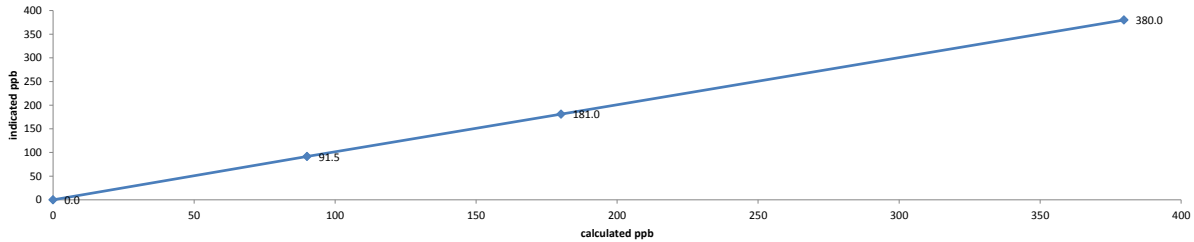

As found:		As left:	
Bkg:	86.1	Bkg:	82.7
Coef:	0.933	Coef:	0.916
Pmt:	-654	Pmt:	-654
0	Lamp=848	0	Lamp=847
Battery:	3.3	Battery:	3.3
Internal:	29.6	Internal:	27.0
Chamber:	45.3	Chamber:	45.3
Pressure:	414.2	Pressure:	414.6
Flow:	0.720	Flow:	0.725
Intensity:	37780	Intensity:	38042
Averaging Time:	120	Averaging Time:	120
Expected Value:	256.7	Expected Value:	249.7

Comments: The analyzer sample inlet filter was changed. The analyzer cooling fan filter(s) were cleaned. The manifold blower was found to be working normally.

SO2[ppb] Station: PRAMP\_986 Daily: 18/10/11 Type: AVG 1 Min. [1 Min.]

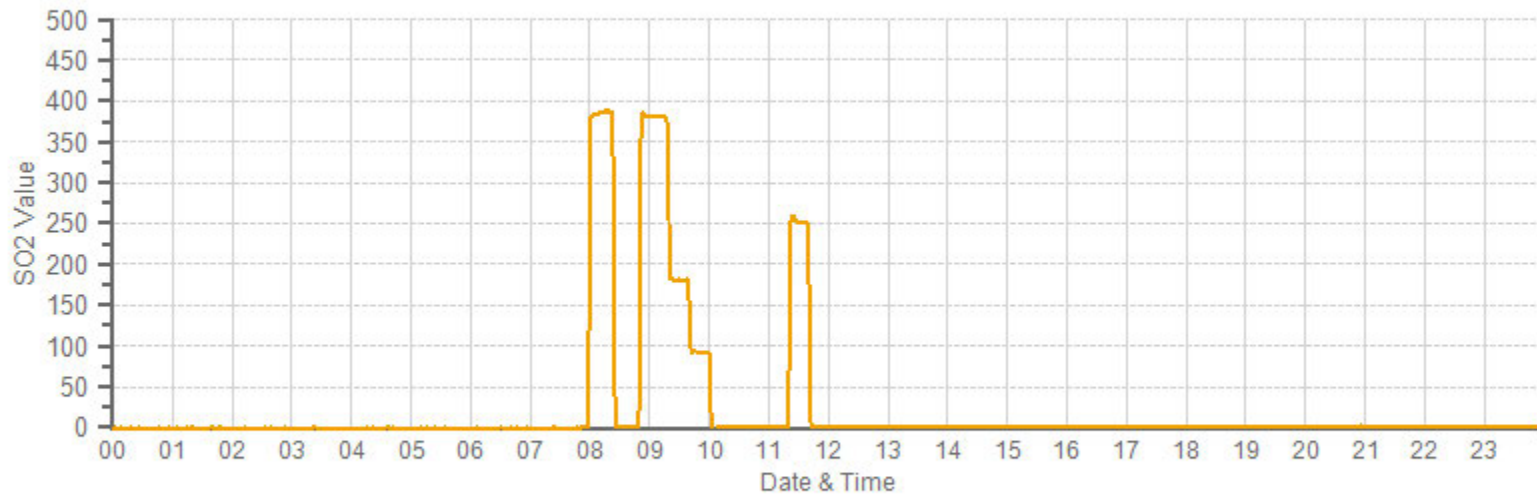

— SO2[ppb]

***TOTAL REDUCED SULPHUR***



### Thermo 431-TLE Total Reduced Sulphur Analyzer Calibration

Date:	October 10, 2018	Barometer/B.P./units:	Brunton 05535 expires December 15, 2018	28.06	inHg
Company/Airshed:	PRAMP	Thermometer/Station Temp:	F.S. 160459244 expires June 19, 2020	21	°C
Location/Station Name:	986B	Weather Conditions:	Cloudy/Overcast		
Parameter:	Total Reduced Sulphur	Calibration Purpose:	routine monthly		
Start Time 24 hr. (mst):	15:15	Performed By/Reviewer:	Limin Li	Rob Fisher	
End Time 24 hr. (mst):	19:27	Cal Gas Expiry Date:	August 23, 2020		
Calibration Method:	Gas Dilution	Converter Model & s/n (if applicable):	CD Nova CDN-101 #516		
Analyzer:					
Serial Number/Owner:	1152940011   Maxxam	Range ppb:	100		
Last Calibration Date:	September 11, 2018	As Found C.F.:	1.037		
Previous C.F.:	0.999	New C.F.:	1.002		

<b>Calibration Standards:</b> Low Flow Meter ID/Expiry Date: Defender Low 152020 expires November 22, 2018 High Flow Meter ID/Expiry Date: Defender High 148943 expires November 21, 2018 Calibrator ID/Expiry Date: Envionics id# 1991 expires March 15, 2019 Cal Gas Cylinder I.D. #: LL119500 Cal Gas Conc. (ppm): 9.8	<b>Standard Calibration Points for Ranges</b> <table border="1"> <tr><th>Point</th><th>ppb</th></tr> <tr><td>High</td><td>78</td></tr> <tr><td>Mid</td><td>38</td></tr> <tr><td>Low</td><td>19</td></tr> </table>	Point	ppb	High	78	Mid	38	Low	19	<b>SO2 Scrubber Check (10 minutes):</b> Start/End Time 24 hr.: 15:18/15:35 SO2 Analyzer Range: 500 Target Concentration (ppb): 380 As Found Zero: 0.1 Analyzer Response (ppb): 0.2 Zero Corrected Result (ppb): 0.1
Point	ppb									
High	78									
Mid	38									
Low	19									


ALL POINTS ARE 15 MINUTES OF STABILITY AS OF SEPTEMBER 23, 2015

Calibrator Flow Rates (cc/min)				Calculated	Indicated Concentration (ppb):	Correction Factors (C.F.):
Point	Diluent	Cal Gas	Total	Concentration (ppb):		
as found zero	7478	0.00	7478	0.0	0.13	n/a
as found high	7410	59.78	7470	78.4	75.77	1.037
adjusted zero	7499	0.00	7499	0.0	0.00	n/a
adjusted high	7445	59.77	7505	78.0	77.90	1.002
mid	7465	29.07	7494	38.0	37.62	1.011
low	7486	14.55	7501	19.0	18.50	1.028
calibrator zero	7499	0.00	7499	0.0	0.10	n/a
Average C.F. =						1.013

Linear Regression/Calibration Results:

Correlation Coefficient =	1.000	LIMITS	> or = 0.995
Slope =	1.000		0.95-1.05
b (Intercept as % of full scale) =	0.26%		± 3% F.S.
% change in C.F. from last cal =	-3.79%		± 10%


Thermo 431-TLE Total Reduced Sulphur Analyzer Calibration

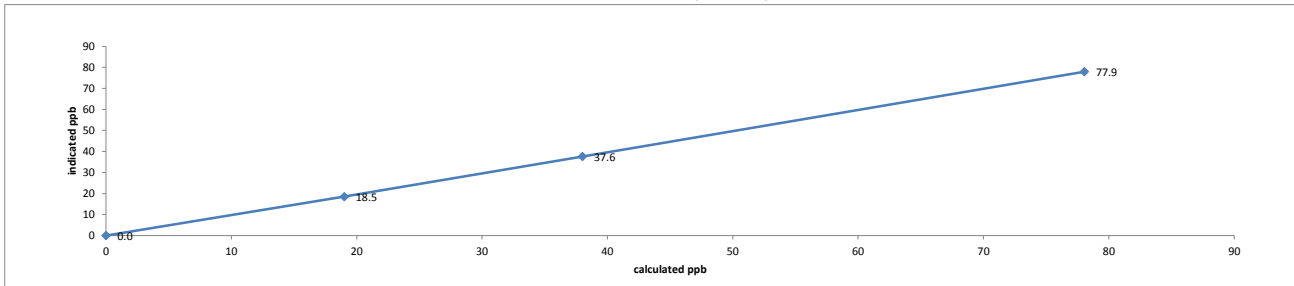

As found:		As left:	
Bkg:	1.79	Bkg:	2.07
Coef:	0.924	Coef:	0.968
Pmt:	-691.2	Pmt:	-691.2
Flash:	963	Flash:	965
Internal:	29.9	Internal:	32.2
Chamber:	45.0	Chamber:	45.0
Perm Oven Gas:	45.00	Perm Oven Gas:	45.00
Perm Oven Heater:	44.24	Perm Oven Heater:	44.25
Pressure:	665.0	Pressure:	664.7
Sample Flow:	0.485	Sample Flow:	0.485
Lamp Intensity:	91	Lamp Intensity:	91
Converter:	820	Converter:	820
Converter Set:	820	Converter Set:	820
Averaging Time:	120	Averaging Time:	120
Expected Value:	41.8	Expected Value:	41.2

Comments: The analyzer sample inlet filter was changed. The analyzer cooling fan filter(s) were cleaned. The manifold blower was found to be working normally.

TRS[ppb] Station: PRAMP\_986 Daily: 18/10/10 Type: AVG 1 Min. [1 Min.]

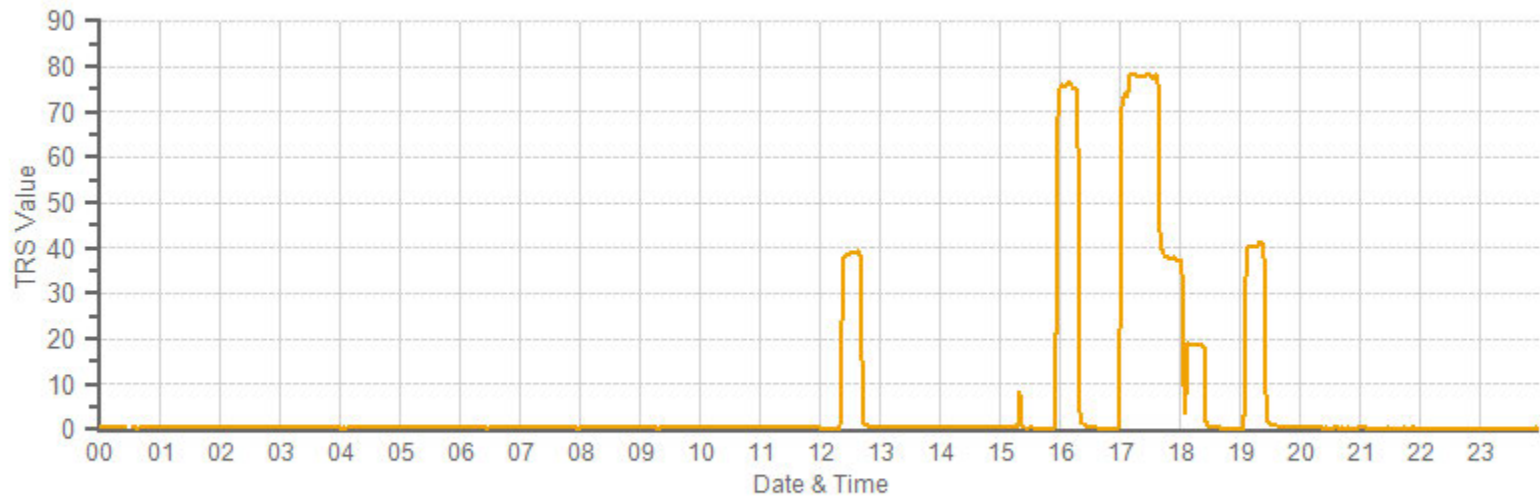

— TRS[ppb]



***TOTAL HYDROCARBON***



### Thermo 55i Methane/Non-Methane Analyzer Calibration

<b>Date:</b>	October 10, 2018	<b>Barometer/B.P./units:</b>	Brunton 05535 expires December 15, 2018	28.06	inHg
<b>Company/Airshed:</b>	PRAMP	<b>Thermometer/Station Temp:</b>	F.S. 160459244 expires June 19, 2020	21	°C
<b>Location/Station Name:</b>	986B	<b>Weather Conditions:</b>	Cloudy/Overcast		
<b>Parameter:</b>	CH4 / NMHC / THC	<b>Calibration Purpose:</b>	routine monthly		
<b>Start/End Time 24 hr. (mst):</b>	15:15/18:39	<b>Performed By/Reviewer:</b>	LIMIN LI	Rob Fisher	
<b>Calibration Method:</b>	Gas Dilution	<b>Cal Gas Expiry Date:</b>	October 18, 2025		

<b>Analyzer:</b>	<b>Serial Number/Owner:</b> 1022143392   Maxxam	<b>Correction Factors:</b>		
<b>Measured Flow:</b> 978 sccm	<b>Last Calibration Date:</b> September 11, 2018	<b>Previous C.F.:</b>	<b>As Found C.F.:</b>	<b>New C.F.:</b>
<b>Range ppm:</b> 20 CH4/20 NMHC/40 THC		CH <sub>4</sub> = 0.998	0.978	1.001
		NMHC = 1.003	0.974	0.999
		THC = 1.000	0.976	1.000

**Calibration Standards:**

<b>Low Flow Meter ID/Expiry Date:</b>	n/a	<b>Standard Calibration Points for Analyzer Range of 20/20/40 ppm</b>			
<b>High Flow Meter ID/Expiry Date:</b>	n/a	<b>Point</b>	<b>CH4</b>	<b>NMHC</b>	<b>THC</b>
<b>Calibrator ID/Expiry Date:</b>	Sabio id# 17200415 expires August 21, 2019	<b>High</b>	<b>13.00</b>	<b>13.00</b>	<b>26.00</b>
<b>Cal Gas Cylinder I.D. #:</b>	LL168404	<b>Mid</b>	<b>7.00</b>	<b>7.00</b>	<b>14.00</b>
<b>CH4 Cylinder Conc.:</b> 597.0	206.0 = C <sub>2</sub> H <sub>6</sub> Cylinder Conc.	<b>Low</b>	<b>3.00</b>	<b>3.00</b>	<b>6.00</b>
<b>CH<sub>4</sub> expressed as C<sub>2</sub>H<sub>6</sub>:</b> 566.5	1163.5 = total CH4 equivalent				

ALL POINTS ARE 15 MINUTES OF STABILITY AS OF SEPTEMBER 23, 2015

Point	Calibrator Flow Rates (cc/min)			Calculated CH <sub>4</sub> (ppm)	Calculated NMHC (ppm)	Calculated THC (ppm)	Indicated CH <sub>4</sub> (ppm)	Indicated NMHC (ppm)	Indicated THC (ppm)	Correction Factors:		
	Diluent	Cal Gas	Total Flow							CH <sub>4</sub>	NMHC	THC
as found zero	3500	0.00	3500	0.00	0.00	0.00	0.00	0.00	0.00	n/a	n/a	n/a
as found high	3414	84.20	3498	14.37	13.64	28.01	14.70	14.00	28.70	0.978	0.974	0.976
adjusted zero	3500	0.00	3500	0.00	0.00	0.00	0.00	0.00	0.00	n/a	n/a	n/a
adjusted high	3414	84.20	3498	14.37	13.64	28.01	14.36	13.65	28.01	1.001	0.999	1.000
mid	3456	42.10	3498	7.19	6.82	14.00	7.23	6.85	14.08	0.994	0.995	0.995
low	3477	21.10	3498	3.60	3.42	7.02	3.63	3.44	7.07	0.992	0.993	0.993
calibrator zero	3500	0.00	3500	0.00	0.00	0.00	0.00	0.00	0.00	n/a	n/a	n/a
<b>Average C.F. =</b>										0.996	0.996	0.996

**Linear Regression/Calibration Results:**

<b>Correlation Coefficient =</b>	CH <sub>4</sub>	NMHC	THC	<b>LIMITS</b> > or = 0.995 0.95-1.05 ± 3% F.S. ± 10%
<b>Slope =</b>	1.000	1.000	1.000	
<b>b (Intercept as % of full scale) =</b>	0.999	1.001	1.000	
<b>% change in C.F. from last cal =</b>	0.11%	0.06%	0.09%	




**As Left Instrument Diagnostics:**


<b>Interface Board Voltages:</b>	Bias Supply: -311.0	<b>Calibration History cnt'd:</b>	NM Peak Area: 76948
<b>Temperatures:</b>	Detector Oven: 175.1	<b>Crucial Settings:</b>	Methane Start: 8
	Filter: 175.1		Methane End: 16
	Column Oven: 75.0		Backflush: 18
	Internal: 34		NMHV Start: 26
<b>Cylinder Pressures/reg.:</b>	Carrier: 2300   50	<b>Run History&gt;1:</b>	NMHC End: 56
	Fuel: 1650   50		Date: 10OCT18
	Span Gas: 900   24		Time: 15:34
	Zero Air Generator: 50		CH <sub>4</sub> PK RT: 0
<b>Internal Pressures:</b>	Carrier: 31.3		CH <sub>4</sub> RT: 12.4
	Fuel: 40.5		CH <sub>4</sub> Baseline: 1634
	Air: 30.8		CH <sub>4</sub> LOD: 17
<b>FID Status:</b>	Status: LIT		CH <sub>4</sub> SD: 5
	Counts: 20235		CH <sub>4</sub> CONC: 0.00
	Flame: 321.1		NM PK HT: 0
	Det Base: 175		NM Peak Area: 0
<b>Flame and Power Stats:</b>	Last Power On: 01OCT18 09:30		NM CONC: 0.00
	Flameouts: 1		NM Base Start: 1618
	Det Oven at Start: 169.5		NM Base End: 1623
	Col Oven at Start: 74.8		NM LOD: 6
<b>Calibration History:</b>	Time: 10OCT18 16:29		NM Start IDX: 4
	Type: SPAN		NM End IDX: 38
	Status: GOOD		NM Max Slope: 4.5e-01
	Check/Adjust: ADJUST		NM Min Slope: -2.4e-01
	CH <sub>4</sub> Span Conc: 14.37		NM PT Count: 0
	CH <sub>4</sub> SP Ratio: 0.000736	<b>Expected Values:</b>	Previous CH <sub>4</sub> : 10.21
	CH <sub>4</sub> RT: 12.4		Previous NMHC: 11.06
	CH <sub>4</sub> PK IDX: 22		Previous THC: 21.14
	CH <sub>4</sub> PK HT: 19514		New CH <sub>4</sub> : 10.21
	NM Span Conc: 13.64		New NMHC: 11.06
	NM SP Ratio: 0.000177		New THC: 21.14

**Comments:**  
 The analyzer sample inlet filter was changed.  
 No zero adjustment was required/made. As found zero values were copied to adjusted zero values for linearity calculation purposes.  
 The analyzer cooling fan filter(s) were cleaned.  
 The manifold blower was found to be working normally.

Date: October 10, 2018  
Company/Airshed: PRAMP  
Location/Station Name: 986B

Start/End Time 24 hr. (mst): 15:15/18:39  
Calibration Purpose: routine monthly  
Calibration Method: Gas Dilution

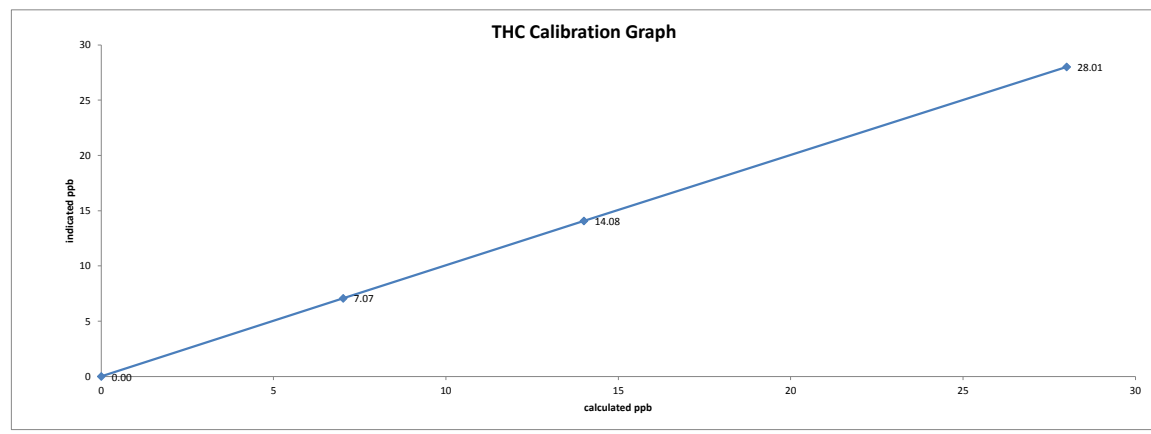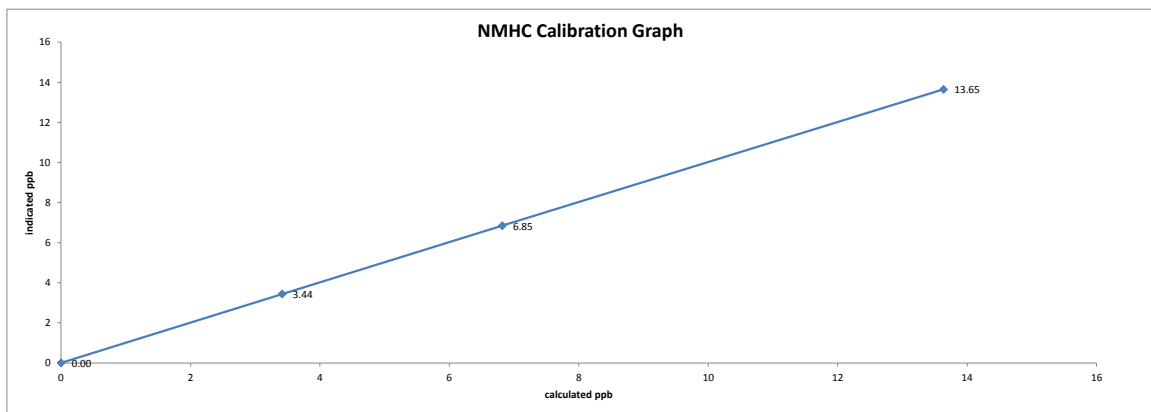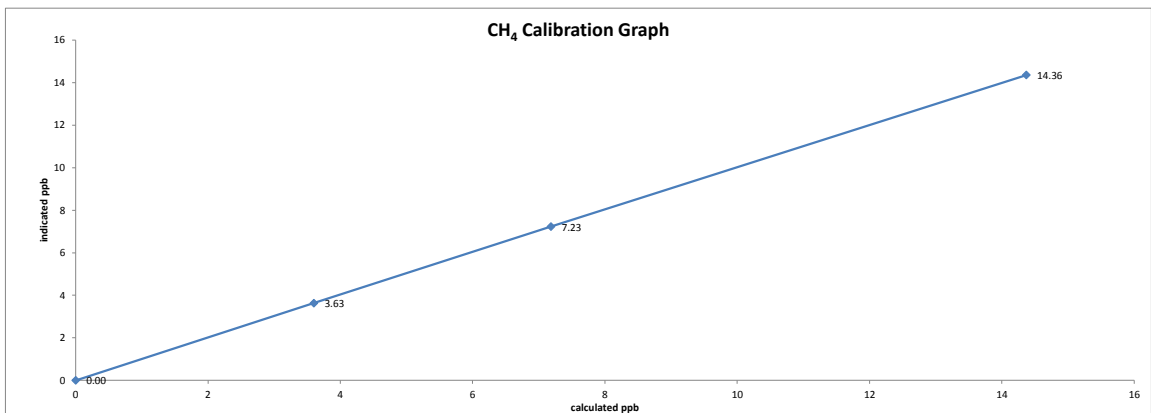

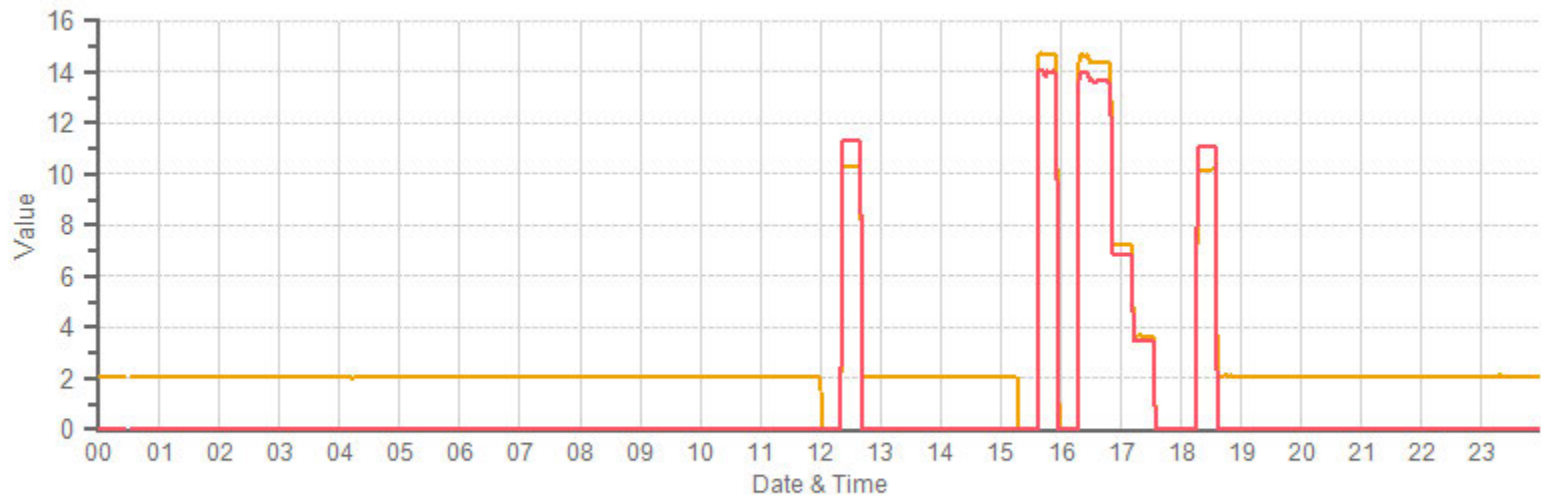

— CH4[ppm] — NMHC[ppm]

## ***WIND SYSTEM***



# Meteorological Sensor Audit/Calibration

## Location Information

Company:	PRAMP	Performed By:	Limin Li
Audit Location:	986B	Reviewed By:	Tom Bourque
Audit Date:	April 4, 2018	Start/End Time (mst):	16:22/17:42
Calibration Purpose:	routine annual	Weather Conditions:	Mainly sunny

## Wind Sensor Information

Sensor ID Data:		Sensor Outputs:	
Sensor Make:	RM Young	Velocity Voltage Output Range:	0-1V
Sensor Model:	5305VK	Velocity Unit Output Range:	0-200 KPH
Serial #:	129612	Direction Voltage Output Range:	0-1 V
Previous Cal/Audit Date:	April 5, 2017	Direction Unit Output Range:	0-360 DEG

## Wind Calibrator Information

Calibrator I.D. and Expiry Date: RM Young 18802 id# CA03309 expires September 25, 2018

### Wind Speed Audit Data **\*\*+/- 2% of the average correction factor is the limit\*\***

RPM	Wind Speed Generated kph	Clockwise Wind Speed kph	Counter Clockwise Wind Speed kph	Correction Factor
0	0	0.1	0.1	-
1000	18.4	18.5	18.5	0.996
2000	36.9	36.9	36.9	1.001
3000	55.3	55.3	55.3	1.000
4000	73.7	73.7	73.7	1.000
5000	92.2	92.2	92.2	1.000
6000	110.6	110.7	110.7	0.999
7000	129.0	129.2	129.2	0.998
8000	147.4	147.7	147.7	0.998
9000	165.9	166.2	166.2	0.998
10000	184.3	184.8	184.8	0.997
The audit meets AMD requirements.			Average Correction Factor=	<b>0.999</b>

### Wind Direction Audit Data **\*\*+/- 3° of the absolute average degrees difference for all points is the limit\*\***

Generated Wind Direction 0-360 (Up)	Generated Wind Direction 360-0 (Down)	Indicated Wind Direction 0-360 (Up)	Indicated Wind Direction 360-0 (Down)	Degrees Difference 0-360 (Up)	Degrees Difference 360-0 (Down)	Average Absolute Degrees Difference
0	355	0	354	0.3	1.4	0.8
30	330	30	330	0.2	0.1	0.1
60	300	61	301	-0.7	-0.9	0.8
90	270	91	271	-1.1	-1.2	1.1
120	240	122	243	-1.7	-2.6	2.2
150	210	153	213	-2.5	-2.9	2.7
180	180	183	183	-2.6	-2.6	2.6
210	150	213	152	-2.6	-1.7	2.1
240	120	243	122	-2.8	-2.0	2.4
270	90	272	91	-2.3	-1.1	1.7
300	60	301	62	-0.8	-1.7	1.2
330	30	331	30	-0.5	-0.3	0.4
355	0	354	0	1.3	0.3	0.8
The audit meets AMD requirements.				Average Absolute Degrees Difference=		<b>1.5</b>

Comments:

***METEOROLOGICAL SYSTEMS CHECK***



## Meteorological System Checklist

Date:	October 10, 2018		
Technician:	Limin Li		
Reviewer:	Rob Fisher		
Station:	PRAMP 986B		
<b>Unit:</b>	<b>Make:</b>	<b>Model:</b>	<b>Serial #:</b>
Temperature Sensor:	RM Young	43172VC	61012322
Barometric Pressure Sensor:	MetOne	090D	F3845
Relative Humidity Sensor:	RM Young	43172VC	61012322
Anemometer:	RM Young	05305VK	129612
<b>AMBIENT TEMPERATURE SENSOR CHECK</b>			
Previous check date:	September 11, 2018		
Parameter:	Temperature @ 2 metres (1 C tolerance)		
Reference Thermometer ID:	F.S. 160459244 expires June 19, 2020		
Reference Temperature (°C):	-0.1		
Station - Ambient Temperature (°C):	-0.2		
Temperature Difference (°C):	0.1		
<b>BAROMETRIC PRESSURE SENSOR CHECK</b>			
Previous check date:	September 11, 2018		
Reference Barometer ID:	Brunton 05535 expires December 15, 2018		
Reference Pressure - Units/Reading:	inHg	28.05	
Station Pressure - Units/Reading:	inHg	28.015	
Pressure Tolerance +/- 15% of error:	24 - 32	0.12%	
<b>RELATIVE HUMIDITY (HYGROMETER) SENSOR CHECK</b>			
Previous check date:	September 11, 2018		
Reference Hygrometer ID:	F.S. id# 160459244 expires June 19, 2020		
Reference Hygrometer % RH- Reading:	72.50		
Station Hygrometer % RH- Reading:	78.30		
RH Tolerance +/- 15% of difference:	61.63 - 83.38	-8.0%	
<b>ANEMOMETER - WIND SPEED &amp; WIND DIRECTION SENSOR CHECK</b>			
<b>WIND SPEED</b>		<b>WIND DIRECTION</b>	
Previous check date:	September 11, 2018	Previous check date:	September 11, 2018
Wind Speed Observed (kph):	0 ~ 5	Wind Direction Observed:	NW
Wind speed on Data Logger (kph):	2	Wind Direction on Data Logger:	NW
		Wind Direction Pass/Fail?:	Pass



## ***CALIBRATORS***

Company <u>Maxxam</u>		Operator: <u>Mike</u>	
<b>Calibrator:</b>		<b>Flow Measurement Device:</b>	
Make/Model	<u>Sabio</u>	Make/Model	<u>Bios Definer 220</u>
Serial Number	<u>17200415</u>	Serial Number	<u>H=128686; L=129069</u>
Last Verification Date	<u>May 16, 2017</u>	Temperature (°C)	<u>22.2 C</u>
NO Cylinder S/N	<u>LL104183</u>	Barometric Pressure	<u>706.1mmHg</u>
NO [PPM]	<u>50.8</u>	NOx [PPM]	<u>50.9</u>
Expiry Date	<u>October 24, 2020</u>		

Dilution Flow (sccm)			
Pt. #1	<u>5057</u>	Pt. #2	<u>5055</u>
		Pt. #3	<u>5070</u>
Gas Flow (sccm)			
Pt. #1	<u>77.4</u>	Pt. #2	<u>37.9</u>
		Pt. #3	<u>19.1</u>

Calibrator Flow (sccm)		Calculated Conc.(ppm)		Indicated Conc.(ppm)			% Difference vs Audit Gas	
Dilution	Gas	NO	NOx	NO	NO <sub>2</sub>	NOx	NO	NOx
5102	0.0	0.0000	0.0000	0.0001	-0.0002	-0.0001	Limit ± 10%	
5057	77.4	0.7775	0.7779	0.7973	0.0012	0.7985	3%	3%
5055	37.9	0.3809	0.3816	0.3896	0.0000	0.3896	2%	2%
5070	19.1	0.1914	0.1918	0.1962	0.0000	0.1962	2%	2%
Absolute Average Percent Difference							2%	2%

**LINEAR REGRESSION ANALYSIS** *y=mx+b (where x=calculated concentration, y=indicated concentration)*

<b>NO</b>	<b>LIMITS</b>	<b>NOx</b>
Correlation= 1.0000	≥ 0.990	Correlation= 1.0000
m (Slope)= 1.0253	<b>0.90-1.10</b>	m (Slope)= 1.0266
b (Intercept % of FS)= -0.0176	± 3% F.S.	b (Intercept % of FS)= -0.0763

Flow	O <sub>3</sub> Conc	NO Decrease	NO	NO <sub>2</sub>	NOX	% Diff. Vs Audit gas	
5057	0.0	0.0000	0.7868	0.0006	0.7874	NO <sub>2</sub>	% Diff. Limit
5057	500.0	0.5003	0.2865	0.5016	0.7875	0%	± 10%
5057	275.0	0.2802	0.5066	0.2797	0.7862	0%	± 10%
5057	100.0	0.1053	0.6815	0.1046	0.7863	-1%	± 10%
Absolute Average Percent Difference						0%	± 10%

**LINEAR REGRESSION ANALYSIS** *y=mx+b (where x=calculated concentration, y=indicated concentration)*

<b>NO<sub>2</sub></b>	<b>LIMITS</b>	
Correlation= 1.0000	≥ 0.995	
m (Slope)= 1.0020	<b>0.90-1.10</b>	
b (Intercept % of FS)= -0.0259	± 3% F.S.	

<b>AENV Standards</b>	<b>NO<sub>x</sub> Analyzer</b>
<b>Audit Calibrator</b>	
Make/Model	<u>Thermo 146i</u>
Serial/AMU Number	<u>1809</u>
SRM Gas Cylinder No.	<u>APEX1170572</u>
Cylinder Conc. (ppm)	<u>49.99</u>
	Make/Model
	<u>Thermo 42i</u>
	Serial/AMU Number
	<u>1868</u>
	Last Calibration Date
	<u>August 16, 2018</u>
	Full Scale (ppm)
	<u>1.0</u>
	Cylinder Gas Expiry Date
	<u>November 15, 2020</u>

COMMENTS:

Auditor: Shea Beaton  
Operator Signature: 

Date: August 21, 2018  
Location: McIntyre Center Edmonton

<b>Company:</b> <u>Maxxam</u>		<b>Operator:</b> <u>Chris W</u>	
<b>Calibrator:</b>		<b>Flow Measurement Device:</b>	
Make/Model	<u>EnviroNics 2000</u>	Make/Model	<u>Mesa Defender 530</u>
Serial Number	<u>1991</u>	Serial Number	<u>L-153351 H-152571</u>
Last Verification Date	<u>March 2017</u>	Temperature (°C)	<u>25.0 C</u>
NO Cylinder S/N	<u>LL108015</u>	Barometric Pressure	<u>695 mmHg</u>
NO [PPM]	<u>52.2</u>	NOx [PPM]	<u>52.3</u>
Expiry Date	<u>Oct 2020</u>		

<b>Dilution Flow (sccm)</b>			
Pt. #1	<u>5000</u>	Pt. #2	<u>5000</u>
Pt. #3	<u>5000</u>		
<b>Gas Flow (sccm)</b>			
Pt. #1	<u>80</u>	Pt. #2	<u>40</u>
Pt. #3	<u>20</u>		

Calibrator Flow (sccm)		Calculated Conc.(ppm)		Indicated Conc.(ppm)			% Difference vs Audit Gas	
Dilution	Gas	NO	NOx	NO	NO <sub>2</sub>	NOx	NO	NOx
5000	0.0	0.000	0.000	0.000	0.000	0.000	Limit ± 10%	
4988	75.1	0.786	0.787	0.785	-0.002	0.783	0%	-1%
4988	36.5	0.382	0.383	0.382	0.001	0.383	0%	0%
4988	18.3	0.192	0.192	0.190	0.000	0.190	-1%	-1%
Absolute Average Percent Difference							0%	1%

**LINEAR REGRESSION ANALYSIS** *y=mx+b (where x=calculated concentration, y=indicated concentration)*

<b>NO</b>	<b>LIMITS</b>	<b>NOx</b>
Correlation= 1.0000	≥ <b>0.990</b>	Correlation= 1.0000
m (Slope)= 0.9996	<b>0.90-1.10</b>	m (Slope)= 0.9956
b (Intercept % of FS)= -0.0599	± <b>3% F.S.</b>	b (Intercept % of FS)= -0.0005

Flow	O <sub>3</sub> Conc	NO Decrease	NO	NO <sub>2</sub>	NOX	% Diff. Vs Audit gas	
4988	0.000	0.000	0.788	-0.001	0.787	NO <sub>2</sub>	% Diff. Limit
4988	0.350	0.519	0.269	0.512	0.780	-1%	± 10%
4988	0.160	0.231	0.557	0.229	0.786	0%	± 10%
4988	0.070	0.099	0.689	0.097	0.787	-1%	± 10%
Absolute Average Percent Difference						1%	± 10%

**LINEAR REGRESSION ANALYSIS** *y=mx+b (where x=calculated concentration, y=indicated concentration)*

<b>NO<sub>2</sub></b>	<b>LIMITS</b>
Correlation= 1.0000	≥ <b>0.995</b>
m (Slope)= 0.9885	<b>0.90-1.10</b>
b (Intercept % of FS)= -0.0567	± <b>3% F.S.</b>

<b>AENV Standards Audit Calibrator</b>	<b>NO<sub>x</sub> Analyzer</b>
Make/Model <u>Teco 146i</u>	Make/Model <u>Teco 42i</u>
Serial/AMU Number <u>AMU 1809</u>	Serial/AMU Number <u>AMU 1868</u>
SRM Gas Cylinder No. <u>APEX1170572</u>	Last Calibration Date <u>March 14, 2018</u>
Cylinder Conc. (ppm) <u>49.99</u>	Full Scale (ppm) <u>1.0</u>
	Cylinder Gas Expiry Date <u>November 2020</u>

COMMENTS: Cylinder contains 47.9 ppm SO2.

Auditor: Al Clark  
Operator Signature:

Date: March 15, 2018  
Location: McIntyre Center Edmonton

## ***CALIBRATION GASES***



# Calibration Gas Audit

## Single Component Cylinder Gas

File No. 2016-436CGA

**Company:** Maxxam **Operator's Name:** Chris

Cylinder #: EY0000769 Concentration PPM: 50.5 Tolerance(%) 1.6 Certified By: Praxair

Expiry Date: December 8, 2019

Reference Calibrator and Gas:	Flow Measurement Device:
Make/Model: <u>Thermo 146i</u>	Make/Model: <u>Bios Befiner 220</u>
Serial Number: <u>AMU 1809</u>	Serial Number: <u>AMU1941</u>
Last Verification Date: <u>January 26, 2017</u>	Temp. °C: <u>24.4</u>
Gas Type: <u>SO2</u> Conc. <u>98.07</u>	B.P. <u>704.7</u>
Cylinder Number: <u>CAL016625</u>	
Expiry Date: <u>January 5, 2019</u>	

**Reference Analyzer:**

Make/Model: Themro 43C Serial/AMU Number: AMU 1623

Instrument Settings: Zero: 9.5 Span: 1.023 Range: 1.0

Last Calibration: Date: 25-Jan-17 C.F. 1.000 Done By: SB

Calibrator Flows (sccm)		Indicated Concentration (PPM)	Gas Flow/ Dilution Flow	Concentration Factor	Cylinder Concentration
Dilution	Gas				
4911	0.0	0.000	<del>0.01574</del>	<del>127.740</del>	<del>50.9</del>
4918	77.4	0.801	0.01574	63.540	50.9
4918	38.5	0.398	0.00783	127.740	50.9
4915	19.2	0.196	0.00391	255.990	50.0
Average Cylinder Concentration:					<b>50.6</b>

Previous Stated Concentration PPM: 50.5

Percent variance from Stated: 0.2

Meets Manufacturer Tolerance. Use manufacturers stated concentration  **COMMENTS:** \_\_\_\_\_

< =5% Outside Manufacturer Tolerance. Use manufacturers concentration  \_\_\_\_\_

> 5% Outside Manufacturer Tolerance. **DO NOT USE** this cylinder  \_\_\_\_\_

Auditor: Shea Beaton

Operator Signature: \_\_\_\_\_

Date: January 26, 2017

Location: McIntyre Center Edmonton



# Calibration Gas Audit

## Single Component Cylinder Gas

File No. 2017-213CGA

**Company:** Maxxam **Operator's Name:** C. Wesson  
**Cylinder #:** LL119500 **Concentration PPM:** 9.8 **Tolerance(%)** 2 **Certified By:** Praxair  
**Expiry Date:** August 2020

**Reference Calibrator and Gas:**  
**Make/Model:** R&R MFC 201  
**Serial Number:** AMU 1690  
**Last Verification Date:** September 22, 2017  
**Gas Type:** H2S **Conc.** 20.43  
**Cylinder Number:** CAL015272  
**Expiry Date:** January 2019

**Flow Measurement Device:**  
**Make/Model:** Mesa Definer 220  
**Serial Number:** H-133034 L-132702  
**Temp. °C:** 23.5 C  
**B.P.** 705 mmhg

**Reference Analyzer:**  
**Make/Model:** Teco 450i **Serial/AMU Number:** 1980  
**Instrument Settings:** **Zero:** 22.4 **Span:** 1.091 **Range:** 0.1  
**Last Calibration:** **Date:** Sep 22/17 **C.F.** 1.000 **Done By:** Al Clark

Calibrator Flows (sccm)		Indicated Concentration (PPM)	Gas Flow/ Dilution Flow	Concentration Factor	Cylinder Concentration
Dilution	Gas				
5000	0.0	0.0000	<del>0.0000</del>	<del>0.0000</del>	<del>0.0000</del>
5114	39.5	0.0734	0.00772	129.468	9.5
5096	18.5	0.0345	0.00363	275.459	9.5
5089	9.5	0.0178	0.00187	535.684	9.5
Average Cylinder Concentration:					<b>9.5</b>

Previous Stated Concentration PPM: 9.8  
 Percent variance from Stated: 3

Meets Manufacturer Tolerance. Use manufacturers stated concentration  **COMMENTS:** \_\_\_\_\_  
 <=5% Outside Manufacturer Tolerance. Use manufacturers concentration   
 > 5% Outside Manufacturer Tolerance. **DO NOT USE** this cylinder

**Auditor:** Al Clark **Date:** September 22, 2017  
**Operator Signature:** *Al Clark* **Location:** McIntyre Center Edmonton





# Calibration Gas Audit

## CH4 / C3H8 Cylinder Gas

File No. 2017-488CGA

**Company:** Maxxam **Operators name:** Mike  
**Cylinder #:** LL168404 **Conc CH4 (PPM)** 597/206 **Tolerance (%)** 2 **Certified By:** Praxair  
**Expiry Date:** October 2025

Reference Calibrator and Gas:				Flow Measurement Device:	
Make/Model	<u>R&amp;R MFC 201</u>			Make/Model	<u>Mesa Definer 220</u>
Serial Number	<u>AMU 1690</u>			Serial Number	<u>H-133034 / L-132702</u>
Last Verification Date	<u>December 13, 2017</u>			Temp. °C	<u>23.1 C</u>
Gas Type	<u>CH4</u>	Conc.	<u>990.4</u>	B.P.	<u>707 mmHg</u>
Cylinder Number	<u>5604875</u>	Expiry Date	<u>July 2021</u>		
Gas Type	<u>C3H8</u>	Conc.	<u>246.5</u>		
Cylinder Number	<u>XF003845B</u>	Expiry Date	<u>July 2022</u>		

**Reference Analyzer:**  
**Make/Model** Teco 55i **Serial/AMU Number:** 2108  
**Instrument Settings** **Zero:** N/A **Span:** N/A **Range:** 20.0  
**Last Calibration:** **Date:** Dec 12/17 **C.F.** 1.000 **Done By:** Al Clark

Calibrator Flows (sccm)		Indicated Conc. (ppm)		Gas Flow/ Dilution Flow	Concentration Factor	Cylinder Concentration	
Dilution	Gas	CH4	C3H8			CH4	C3H8
3500	0.0	0.00	0.00	<del>0.02</del>	<del>45.00</del>	<del>595</del>	<del>208</del>
3618	80.4	13.22	12.69	0.02	45.00	595	208
3547	39.8	6.64	6.42	0.01	89.12	592	208
3560	19.8	3.33	3.23	0.01	179.80	599	211
Average Cylinder Concentration:						<b>595</b>	<b>209</b>

<b>CH4</b>	<b>C3H8</b>
Previous Stated Concentration PPM: <u>597</u>	<u>206</u>
Percent variance from Stated: <u>0</u>	<u>1</u>

**Cylinder gas tolerances based on CH4 only**

Meets Manufacturer Tolerance. Use manufacturers stated concentration  **COMMENTS:**  
 <=5% Outside Manufacturer Tolerance. Use manufacturers concentration   
 > 5% Outside Manufacturer Tolerance. **DO NOT USE** this cylinder

**Auditor:** Al Clark **Date:** December 13, 2017  
**Operator Signature:** *Al Clark* **Location:** McIntyre Center Edmonton

***APPENDIX III***  
***MAXIMUM INSTANTANEOUS DATA***





PEACE RIVER AREA MONITORING PROGRAM COMMITTEE  
Three Creeks 986b Station - October 2018

SULPHUR DIOXIDE Instantaneous Maximum (SO<sub>2</sub> ppb)

HR START (MST)	0:00	1:00	2:00	3:00	4:00	5:00	6:00	7:00	8:00	9:00	10:00	11:00	12:00	13:00	14:00	15:00	16:00	17:00	18:00	19:00	20:00	21:00	22:00	23:00	DAILY	DAILY	24-HR	RDGS.		
HR END (MST)	0:59	1:59	2:59	3:59	4:59	5:59	6:59	7:59	8:59	9:59	10:59	11:59	12:59	13:59	14:59	15:59	16:59	17:59	18:59	19:59	20:59	21:59	22:59	23:59	MIN.	MAX.	AVG.			
DAY 1	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	1	0	0	S	0	0	0	0	1	0	24	
2	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	24	
3	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	0	24	
4	0	0	0	1	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	1	0	24	
5	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	0	0	0	24	
6	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	0	0	0	0	24	
7	0	0	0	0	0	0	0	0	0	0	0	0	1	0	0	S	1	0	0	0	0	0	0	0	0	0	1	0	24	
8	0	0	0	0	0	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	0	0	0	0	0	0	0	24	
9	0	0	0	0	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	0	0	0	0	0	0	0	0	24	
10	0	0	0	0	0	0	0	0	0	0	0	0	S	0	0	0	0	0	0	Y	0	0	0	0	0	0	0	0	23	
11	0	0	0	0	0	0	0	C	C	C	C	S	1	1	2	2	2	2	2	2	2	2	1	1	0	2	1	24		
12	2	1	2	2	2	2	1	2	2	S	1	2	2	2	2	2	2	2	2	2	2	2	1	2	2	2	2	2	24	
13	2	2	2	2	2	2	1	2	2	S	2	2	2	2	2	2	2	2	2	2	2	2	1	2	1	2	1	2	24	
14	2	2	1	2	2	2	2	2	S	2	2	3	2	2	2	2	2	2	2	2	2	2	2	2	2	1	3	2	24	
15	2	2	3	2	2	2	2	S	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	24	
16	2	2	2	2	2	2	S	2	2	2	2	2	2	3	3	2	2	2	2	2	2	2	2	2	2	2	3	2	24	
17	2	2	2	2	2	S	2	2	2	2	2	2	2	3	2	2	2	3	2	2	2	2	2	2	2	2	3	2	24	
18	3	3	2	2	S	3	3	3	2	2	1	2	3	2	2	2	2	1	2	2	2	2	1	1	2	1	3	2	24	
19	2	1	2	S	2	2	2	2	2	2	3	2	2	2	2	2	1	2	2	2	2	2	1	2	2	1	3	2	24	
20	3	2	S	2	2	2	2	2	2	2	2	2	2	2	2	2	1	2	2	1	2	1	1	1	2	1	3	2	24	
21	1	S	2	2	2	2	2	2	2	2	2	1	1	2	3	2	2	2	2	1	2	2	1	2	1	2	1	3	2	24
22	S	2	1	2	1	1	2	2	2	2	2	3	2	2	2	2	2	2	1	2	1	1	2	S	1	3	2	24		
23	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	3	2	2	2	2	2	2	S	1	1	3	2	24		
24	2	2	2	2	2	2	2	2	2	2	1	2	2	2	2	2	1	2	2	2	2	S	2	2	1	2	2	2	24	
25	2	2	2	2	2	2	1	2	2	2	2	2	2	2	2	2	2	2	2	2	2	S	1	2	2	1	2	2	24	
26	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	2	S	2	2	2	2	2	2	2	24	
27	2	3	2	2	2	2	2	1	2	2	2	2	2	2	2	2	2	2	2	S	2	2	2	2	2	1	3	2	24	
28	2	2	2	1	2	2	2	2	2	2	1	2	2	2	2	2	2	2	S	2	2	2	1	2	2	1	2	2	24	
29	2	2	2	2	2	2	2	2	2	2	2	2	3	3	S	3	2	2	2	2	2	2	2	1	1	3	2	24		
30	2	2	2	2	2	2	2	2	2	2	3	2	2	2	3	S	2	2	2	3	2	2	2	2	2	2	3	2	24	
31	2	2	2	2	2	3	2	2	2	2	2	2	2	2	S	2	2	2	2	2	2	2	2	2	2	2	2	2	24	
HOURLY MAX	3	3	3	2	2	3	3	3	2	2	3	3	3	3	3	3	2	3	2	3	2	2	2	2	2	2	2	2	24	
HOURLY AVG	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	1	24	


STATUS FLAG CODES

C	- MONTHLY CALIBRATION	Q	- QUALITY ASSURANCE
C1	- REPEAT CALIBRATION	R	- RECOVERY
Y	- MAINTENANCE	X	- MACHINE MALFUNCTION
S	- DAILY ZERO/SPAN CHECK	G	- OUT FOR REPAIR
S1	- REPEAT ZERO/SPAN CHECK	P	- POWER FAILURE

MONTHLY SUMMARY

NUMBER OF NON-ZERO READINGS:	475
MAXIMUM INSTANTANEOUS VALUE:	3 ppb @ HOUR 11 ON DAY 14
IZS CALIBRATION TIME:	32 hrs
MONTHLY CALIBRATION TIME:	4 hrs
OPERATIONAL TIME:	743 hrs
STANDARD DEVIATION:	1

SULPHUR DIOXIDE Instantaneous Maximum (SO<sub>2</sub> ppb)

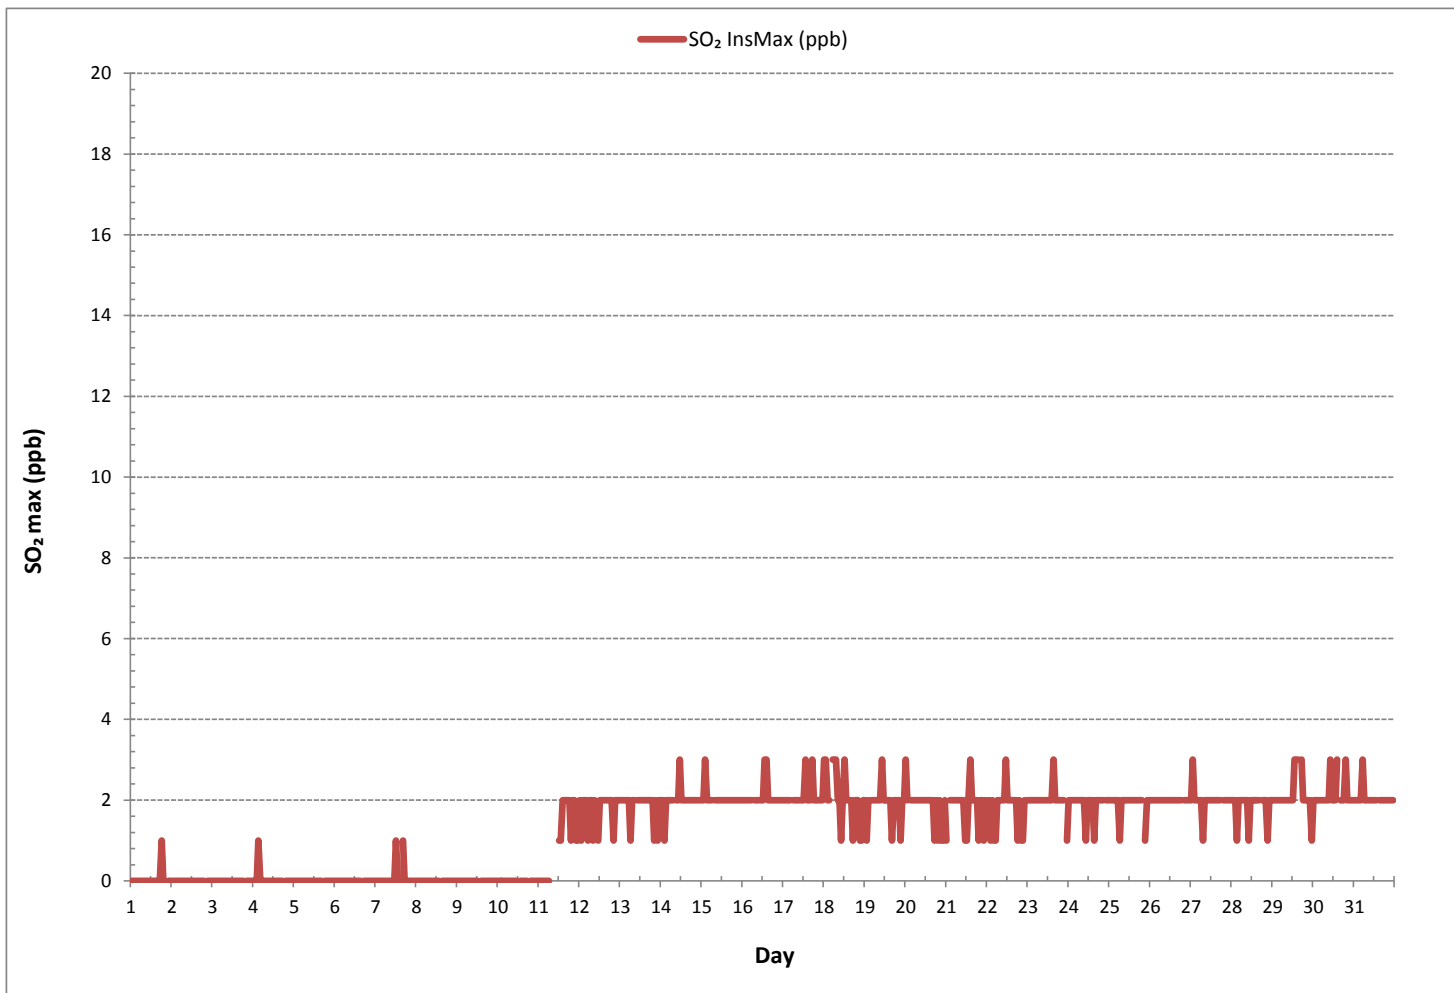



PEACE RIVER AREA MONITORING PROGRAM COMMITTEE  
Three Creeks 986b Station - October 2018

TOTAL REDUCED SULPHUR Instantaneous Maximum (TRS ppb)

HR START (MST)	0:00	1:00	2:00	3:00	4:00	5:00	6:00	7:00	8:00	9:00	10:00	11:00	12:00	13:00	14:00	15:00	16:00	17:00	18:00	19:00	20:00	21:00	22:00	23:00	DAILY	DAILY	24-HR	RDGS.	
HR END (MST)	0:59	1:59	2:59	3:59	4:59	5:59	6:59	7:59	8:59	9:59	10:59	11:59	12:59	13:59	14:59	15:59	16:59	17:59	18:59	19:59	20:59	21:59	22:59	23:59	MIN.	MAX.	AVG.		
DAY 1	0.42	0.43	0.48	0.49	0.47	0.49	0.44	0.47	0.42	0.47	0.42	0.34	0.34	0.34	0.39	0.35	0.34	0.34	0.33	0.36	0.33	S	0.46	0.36	0.33	0.49	0	24	
2	0.37	0.36	0.41	0.41	0.38	0.44	0.46	0.37	0.40	0.40	0.40	0.38	0.37	0.42	0.39	0.39	0.35	0.35	0.36	0.36	S	0.47	0.38	0.38	0.35	0.47	0	24	
3	0.39	0.37	0.41	0.39	0.34	0.40	0.45	0.43	0.38	0.39	0.38	0.37	0.36	0.37	0.36	0.36	0.37	0.36	0.40	S	0.46	0.38	0.37	0.36	0.34	0.46	0	24	
4	0.39	0.35	0.35	0.37	0.38	0.38	0.38	0.38	0.43	0.38	0.38	0.38	0.38	0.40	0.38	0.43	0.37	0.35	S	0.40	0.45	0.42	0.37	0.38	0.35	0.45	0	24	
5	0.38	0.39	0.40	0.41	0.39	0.39	0.38	0.39	0.38	0.38	0.38	0.43	0.36	0.36	0.37	0.37	0.36	S	0.52	0.41	0.37	0.36	0.39	0.39	0.36	0.52	0	24	
6	0.38	0.37	0.40	0.39	0.38	0.39	0.39	0.36	0.37	0.40	0.37	0.36	0.39	0.36	0.37	0.39	S	0.43	0.38	0.42	0.43	0.41	0.35	0.38	0.35	0.43	0	24	
7	0.37	0.40	0.36	0.38	0.38	0.40	0.42	0.36	0.39	0.36	0.40	0.37	0.40	0.42	0.38	S	0.46	0.38	0.37	0.40	0.37	0.40	0.37	0.39	0.36	0.46	0	24	
8	0.40	0.37	0.36	0.38	0.39	0.37	0.40	0.38	0.36	0.35	0.37	0.37	0.36	0.35	S	0.45	0.39	0.39	0.38	0.39	0.37	0.39	0.36	0.39	0.35	0.45	0	24	
9	0.36	0.50	0.39	0.38	0.37	0.40	0.38	0.38	0.37	0.37	0.38	0.38	0.39	S	0.50	0.40	0.40	0.43	0.39	0.40	0.38	0.38	0.37	0.38	0.36	0.50	0	24	
10	0.36	0.35	0.38	0.37	0.36	0.39	0.38	0.37	0.39	0.40	0.42	0.39	S	0.57	0.43	C	C	C	C	C	C	0.39	0.34	0.27	0.27	0.27	0.57	0	24
11	0.29	0.26	0.27	0.25	0.24	0.21	0.25	0.20	0.19	0.16	0.18	S	0.26	0.19	0.22	0.23	0.19	0.21	0.21	0.17	0.16	0.20	0.20	0.22	0.16	0.29	0	24	
12	0.29	0.46	0.29	0.22	0.16	0.15	0.15	0.16	0.15	0.14	S	0.23	0.17	0.22	0.16	0.21	0.20	0.17	0.26	0.33	0.41	0.46	0.60	1.21	1.14	1.21	0	24	
13	1.25	0.46	0.98	0.93	0.76	1.12	0.82	0.74	0.83	S	0.59	0.21	0.19	0.37	0.33	0.22	0.23	0.51	0.66	0.94	0.92	0.45	0.43	0.87	0.19	1.25	1	24	
14	0.82	0.66	0.71	0.51	0.45	0.42	0.40	0.31	S	0.37	0.33	0.30	0.24	0.26	0.30	0.24	0.29	0.28	0.22	0.25	0.25	0.23	0.23	0.50	0.22	0.82	0	24	
15	0.27	0.31	1.12	1.13	0.92	0.85	1.93	S	0.66	0.42	0.50	0.44	0.38	0.26	0.20	0.22	0.18	0.19	0.18	0.76	2.25	3.92	4.04	2.09	0.18	4.04	1	24	
16	2.00	1.55	1.55	1.46	1.29	1.12	S	1.07	0.56	0.61	0.34	0.32	0.30	0.23	0.17	0.19	0.23	0.57	0.39	0.26	0.22	0.22	0.18	0.21	0.17	2.00	1	24	
17	0.20	0.21	0.27	0.23	0.25	S	0.27	0.24	0.21	0.27	0.23	0.21	0.20	0.19	0.17	0.19	0.17	0.20	0.18	0.20	0.19	0.18	0.20	0.15	0.16	0.15	0.27	0	24
18	0.32	0.46	0.47	0.22	S	0.41	0.70	0.66	0.25	0.23	0.18	0.25	0.64	0.22	0.19	0.18	0.20	0.17	0.16	0.18	0.28	0.41	0.53	0.58	0.16	0.70	0	24	
19	0.51	0.57	0.67	S	0.44	0.44	0.57	0.49	0.63	0.43	0.27	0.31	0.22	0.20	0.20	0.21	0.23	0.23	0.24	0.22	0.16	0.21	0.19	0.15	0.15	0.67	0	24	
20	0.18	0.18	S	0.25	0.23	0.18	0.21	0.21	0.20	0.16	0.16	0.21	0.25	0.25	0.19	0.17	0.13	0.16	0.20	0.20	0.15	0.15	0.17	0.13	0.25	0	24		
21	0.14	S	0.30	0.20	0.19	0.29	0.20	0.25	0.34	0.39	0.20	0.20	0.16	0.19	0.23	0.21	0.20	0.21	0.36	0.19	0.20	0.23	0.18	0.25	0.14	0.39	0	24	
22	S	0.35	0.22	0.22	0.24	0.19	0.21	0.19	0.20	0.19	0.20	0.20	0.17	0.18	0.18	0.17	0.27	0.26	0.37	0.27	0.33	0.29	0.26	S	0.17	0.37	0	24	
23	0.46	0.26	0.26	0.30	0.26	0.27	0.37	0.37	0.28	0.37	0.29	0.28	0.20	0.21	0.26	0.25	0.24	0.44	0.44	0.41	0.36	0.35	S	0.41	0.20	0.46	0	24	
24	0.37	0.35	0.30	0.31	0.31	0.51	0.43	0.39	0.34	0.36	0.28	0.24	0.27	0.28	0.28	0.27	0.27	0.33	0.31	0.31	0.26	S	0.34	0.31	0.24	0.51	0	24	
25	0.27	0.31	0.35	0.36	0.26	0.29	0.27	0.25	0.36	0.25	0.21	0.21	0.22	0.24	0.25	0.24	0.24	0.27	0.22	0.22	S	0.26	0.22	0.20	0.20	0.36	0	24	
26	0.17	0.18	0.20	0.20	0.20	0.18	0.27	0.20	0.19	0.23	0.20	0.23	0.20	0.20	0.17	0.19	0.20	0.33	0.22	S	0.63	0.28	0.27	0.21	0.17	0.63	0	24	
27	0.22	0.23	0.19	0.20	0.19	0.27	0.31	0.18	0.20	0.40	0.41	0.17	0.21	0.30	0.15	0.16	0.19	0.43	S	0.68	0.36	0.44	0.38	0.50	0.15	0.68	0	24	
28	0.34	0.41	0.37	0.21	0.50	0.46	0.57	0.57	0.41	0.28	0.24	0.25	0.22	0.16	0.14	0.18	0.20	S	0.33	0.18	0.22	1.01	0.50	0.30	0.14	1.01	0	24	
29	0.55	0.44	0.24	0.23	0.25	0.31	0.66	0.47	0.33	0.34	0.33	0.28	0.24	0.27	0.28	0.31	S	0.44	0.35	0.27	0.20	0.34	0.44	0.31	0.20	0.66	0	24	
30	0.43	0.46	0.55	0.53	0.42	0.49	0.52	0.41	0.33	0.36	0.22	0.24	0.27	0.23	0.21	S	0.33	0.33	0.30	0.30	0.21	0.22	0.23	0.22	0.21	0.55	0	24	
31	0.20	0.28	0.34	0.35	0.29	0.36	0.38	0.35	0.39	0.38	0.20	0.20	0.21	0.17	S	0.32	0.29	0.26	0.24	0.18	0.12	0.16	0.19	0.20	0.12	0.39	0	24	
HOURLY MAX	2.00	1.55	1.55	1.46	1.29	1.12	1.93	1.07	0.83	0.61	0.59	0.44	0.64	0.57	0.50	0.45	0.46	0.57	0.66	0.94	2.25	3.92	4.04	2.09					
HOURLY AVG	0.44	0.41	0.45	0.41	0.39	0.42	0.45	0.39	0.36	0.34	0.32	0.29	0.29	0.28	0.27	0.27	0.27	0.32	0.32	0.34	0.40	0.47	0.45	0.43					


STATUS FLAG CODES

C	- MONTHLY CALIBRATION	Q	- QUALITY ASSURANCE
C1	- REPEAT CALIBRATION	R	- RECOVERY
Y	- MAINTENANCE	X	- MACHINE MALFUNCTION
S	- DAILY ZERO/SPAN CHECK	G	- OUT FOR REPAIR
S1	- REPEAT ZERO/SPAN CHECK	P	- POWER FAILURE

MONTHLY SUMMARY

NUMBER OF NON-ZERO READINGS:	707
MAXIMUM INSTANTANEOUS VALUE:	4.04 ppb @ HOUR 22 ON DAY 15
IZS CALIBRATION TIME:	32 hrs
MONTHLY CALIBRATION TIME:	5 hrs
OPERATIONAL TIME:	744 hrs
STANDARD DEVIATION:	0.29

TOTAL REDUCED SULPHUR Instantaneous Maximum (TRS ppb)

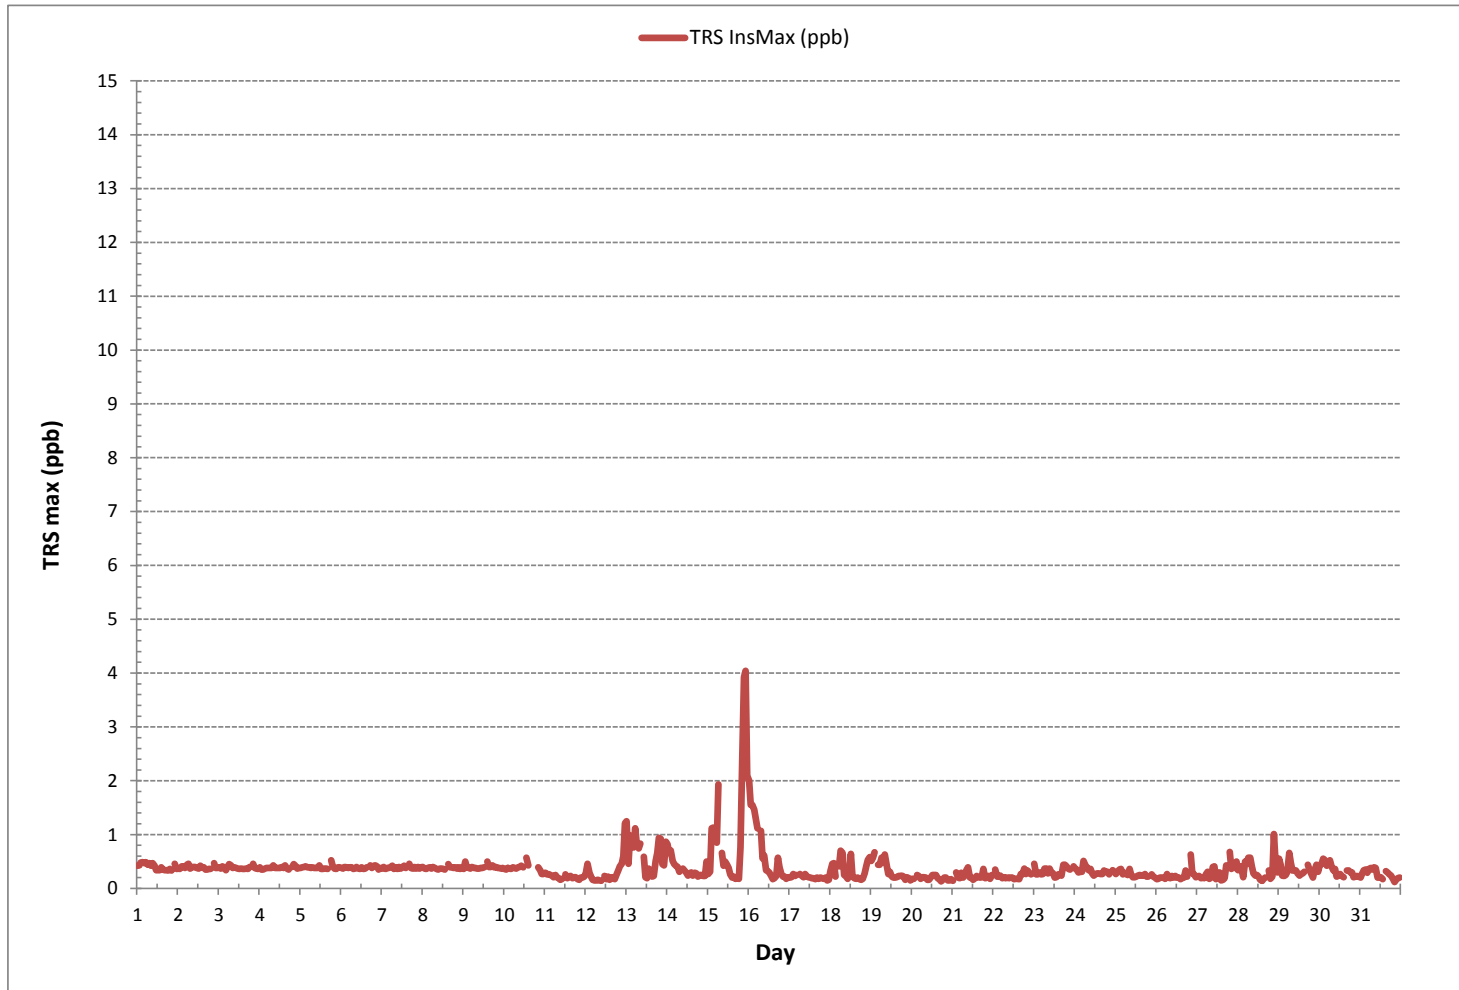



**PEACE RIVER AREA MONITORING PROGRAM COMMITTEE**  
**Three Creeks 986b Station - October 2018**

**TOTAL HYDROCARBONS Instantaneous Maximum (THC ppm)**

HR START (MST)	0:00	1:00	2:00	3:00	4:00	5:00	6:00	7:00	8:00	9:00	10:00	11:00	12:00	13:00	14:00	15:00	16:00	17:00	18:00	19:00	20:00	21:00	22:00	23:00	DAILY MIN.	DAILY MAX.	24-HR AVG.	RDGS.	
HR END (MST)	0:59	1:59	2:59	3:59	4:59	5:59	6:59	7:59	8:59	9:59	10:59	11:59	12:59	13:59	14:59	15:59	16:59	17:59	18:59	19:59	20:59	21:59	22:59	23:59					
DAY																													
1	2.73	2.94	3.18	2.93	2.33	2.30	2.20	2.20	2.11	Y	2.04	2.03	2.02	2.01	2.02	2.02	2.03	2.00	2.03	2.01	2.03	S	2.02	2.03	2.00	3.18	2.24	23	
2	2.10	2.88	2.03	2.03	2.01	2.07	2.16	2.15	2.01	2.12	2.02	2.01	2.01	2.00	2.00	1.99	1.99	1.99	1.99	1.98	S	2.00	2.00	2.02	1.98	2.88	2.07	24	
3	2.82	4.06	2.19	2.08	2.05	2.62	3.17	2.17	2.38	2.02	2.01	1.99	2.02	1.99	2.00	2.00	2.01	S	2.00	2.01	2.02	2.03	1.99	4.06	2.24	24			
4	2.04	2.04	2.01	2.05	2.04	2.01	2.05	2.02	2.05	2.05	2.03	2.01	2.02	2.02	2.02	2.01	2.01	2.00	S	2.03	2.00	2.03	2.02	2.03	2.00	2.05	2.02	24	
5	2.03	2.01	2.03	2.01	2.03	2.00	2.03	2.00	2.00	2.00	2.02	2.02	1.99	2.01	2.00	2.00	2.02	S	2.10	2.04	2.07	2.03	2.02	2.04	1.99	2.10	2.02	24	
6	2.05	2.01	2.03	2.03	2.04	2.02	2.04	2.04	2.03	2.06	2.02	2.05	2.03	2.04	2.04	2.03	S	2.04	2.04	2.04	2.04	2.04	2.03	2.02	2.01	2.06	2.03	24	
7	2.03	2.02	2.03	2.04	2.03	2.05	2.04	2.05	2.04	2.05	2.03	2.05	2.02	2.04	2.01	S	2.03	2.01	2.03	2.01	2.03	2.03	2.03	2.05	2.04	2.01	2.05	2.03	24
8	2.03	2.05	2.02	2.04	2.02	2.04	2.02	2.04	2.00	2.08	2.03	2.01	2.02	2.01	S	2.01	2.01	2.01	2.01	2.03	2.03	2.03	2.03	2.03	2.00	2.08	2.03	24	
9	2.08	2.75	2.08	2.03	2.02	2.04	2.03	2.02	2.03	2.01	2.03	2.01	2.03	S	2.01	2.02	2.02	2.02	2.04	2.06	2.08	2.05	2.03	2.04	2.01	2.75	2.07	24	
10	2.02	2.05	2.04	2.04	2.04	2.02	2.05	2.03	2.06	2.05	2.08	2.05	S	2.06	C	C	C	C	C	2.04	2.03	2.05	2.05	2.17	2.02	2.17	2.05	24	
11	2.07	2.16	2.04	2.19	2.03	2.03	2.04	2.01	2.02	2.00	2.00	S	2.00	2.01	1.98	1.98	1.97	2.00	2.03	2.00	1.97	1.96	1.96	1.94	1.94	2.19	2.02	24	
12	1.97	1.97	1.97	1.96	1.96	1.97	1.97	1.99	1.97	2.00	S	2.02	2.02	2.02	2.06	2.09	2.08	2.11	2.31	2.41	2.61	2.10	2.21	1.99	1.96	2.61	2.08	24	
13	2.57	2.12	1.99	2.00	2.00	2.02	2.04	2.17	2.17	S	2.03	2.02	2.02	1.97	1.98	1.96	1.96	1.96	1.98	1.96	1.99	1.98	1.98	1.98	1.96	2.57	2.04	24	
14	1.99	1.99	1.99	1.99	1.99	1.98	1.97	1.98	S	1.98	1.98	1.97	1.95	1.94	1.95	1.93	1.95	1.93	1.95	1.95	1.98	1.94	2.02	2.13	1.93	2.13	1.97	24	
15	2.31	2.16	2.11	1.94	1.96	1.95	1.96	S	1.95	1.94	2.76	2.02	2.02	2.04	2.05	2.14	2.02	2.27	2.74	2.63	1.95	3.33	2.00	1.97	1.94	3.33	2.18	24	
16	1.98	2.05	2.03	2.08	2.12	2.07	S	2.04	2.00	1.97	1.97	1.96	1.97	1.97	1.97	1.97	1.97	1.96	1.97	1.96	1.95	1.94	1.96	1.95	1.94	2.12	1.99	24	
17	1.94	1.94	1.94	1.93	1.93	S	1.94	1.94	1.96	1.98	1.96	1.97	1.96	1.96	1.93	1.93	1.94	1.93	1.95	1.94	1.98	1.95	1.92	1.96	1.92	1.98	1.95	24	
18	2.07	1.96	1.96	2.26	S	1.94	2.07	2.09	2.13	2.22	2.06	2.13	2.06	1.99	2.07	2.06	2.04	2.39	2.78	2.34	2.08	2.08	2.13	2.13	1.94	2.78	2.13	24	
19	2.08	2.06	2.07	S	2.15	2.08	2.09	2.07	2.11	2.10	2.05	2.01	1.99	1.98	1.97	1.95	1.95	1.96	1.99	1.98	1.97	1.99	1.99	1.97	1.95	2.15	2.02	24	
20	1.95	1.97	S	1.99	1.98	1.96	2.11	1.97	1.95	1.96	1.98	2.00	2.03	2.00	2.00	1.97	1.95	1.95	1.99	2.01	1.95	1.99	2.00	1.96	1.95	2.11	1.98	24	
21	1.96	S	1.97	1.97	1.98	1.98	1.98	2.25	2.25	2.04	2.06	2.20	2.18	2.08	2.04	2.00	2.06	1.99	1.97	1.98	1.99	1.99	2.03	2.11	1.96	2.25	2.05	24	
22	S	2.09	2.11	2.07	2.04	2.02	2.00	2.04	2.17	2.18	1.98	1.96	1.98	1.96	1.97	1.97	1.96	2.21	2.02	2.08	2.08	2.07	2.07	S	1.96	2.21	2.05	24	
23	2.08	2.07	2.10	2.10	2.06	2.31	2.18	2.51	2.14	2.13	2.07	2.07	2.07	2.23	2.34	2.34	2.71	2.37	2.17	2.13	2.16	2.20	S	2.19	2.06	2.71	2.21	24	
24	2.24	2.24	2.23	2.20	2.20	2.45	2.41	2.53	2.55	2.43	2.24	2.09	2.06	2.06	2.05	2.08	2.08	2.09	2.10	2.10	S	2.09	2.08	2.05	2.55	2.20	24		
25	2.11	2.17	2.19	2.09	2.10	2.10	2.03	2.03	2.04	2.00	1.99	1.98	1.97	1.95	1.96	1.94	2.00	1.94	1.96	1.94	S	1.94	1.94	1.94	1.94	2.19	2.01	24	
26	1.96	1.95	1.98	1.96	1.96	1.97	2.02	1.96	1.96	1.98	1.97	1.95	1.95	1.94	1.94	1.93	1.95	1.99	1.96	S	2.01	1.97	1.98	1.99	1.93	2.02	1.97	24	
27	2.00	2.07	1.98	1.95	1.97	2.00	1.98	1.99	1.97	2.01	2.02	1.98	2.10	2.04	2.01	2.05	2.35	1.97	S	2.00	1.96	2.00	2.00	2.01	1.95	2.35	2.02	24	
28	2.03	2.08	2.08	2.08	2.37	2.64	2.10	2.05	2.04	2.01	2.00	1.98	1.97	1.96	1.95	1.96	1.95	S	1.97	3.35	4.29	2.47	2.09	2.50	1.95	4.29	2.26	24	
29	2.52	2.01	2.15	2.10	2.05	1.99	2.03	2.84	2.04	2.05	2.05	2.04	2.02	2.01	2.00	2.02	S	2.00	2.00	1.99	2.00	2.01	2.04	2.02	1.99	2.84	2.09	24	
30	2.04	2.06	2.06	2.06	2.07	2.02	2.01	2.01	2.01	2.01	2.01	2.00	1.98	1.98	1.96	S	1.98	1.96	1.98	1.98	1.99	1.97	1.96	1.98	1.96	2.07	2.00	24	
31	1.99	2.00	1.99	1.98	1.99	2.01	2.03	2.00	1.98	1.98	1.98	1.98	1.97	2.01	S	2.20	2.19	2.06	1.99	2.00	2.03	2.01	2.07	2.04	1.97	2.20	2.02	24	
HOURLY MAX	2.82	4.06	3.18	2.93	2.37	2.64	3.17	2.84	2.55	2.43	2.76	2.20	2.18	2.23	2.34	2.34	2.71	2.39	2.78	3.35	4.29	3.33	2.21	2.50					
HOURLY AVG	2.13	2.20	2.09	2.07	2.05	2.09	2.09	2.11	2.07	2.05	2.05	2.02	2.01	2.01	2.01	2.02	2.04	2.04	2.07	2.10	2.12	2.07	2.02	2.04					


**STATUS FLAG CODES**

C	- MONTHLY CALIBRATION	Q	- QUALITY ASSURANCE
C1	- REPEAT CALIBRATION	R	- RECOVERY
Y	- MAINTENANCE	X	- MACHINE MALFUNCTION
S	- DAILY ZERO/SPAN CHECK	G	- OUT FOR REPAIR
S1	- REPEAT ZERO/SPAN CHECK	P	- POWER FAILURE

**MONTHLY SUMMARY**

NUMBER OF NON-ZERO READINGS:	707
MAXIMUM INSTANTANEOUS VALUE:	4.29 ppm @ HOUR 20 ON DAY 28
IZS CALIBRATION TIME:	32 hrs
MONTHLY CALIBRATION TIME:	4 hrs
OPERATIONAL TIME:	743 hrs
STANDARD DEVIATION:	0.20

TOTAL HYDROCARBONS Instantaneous Maximum (THC ppm)

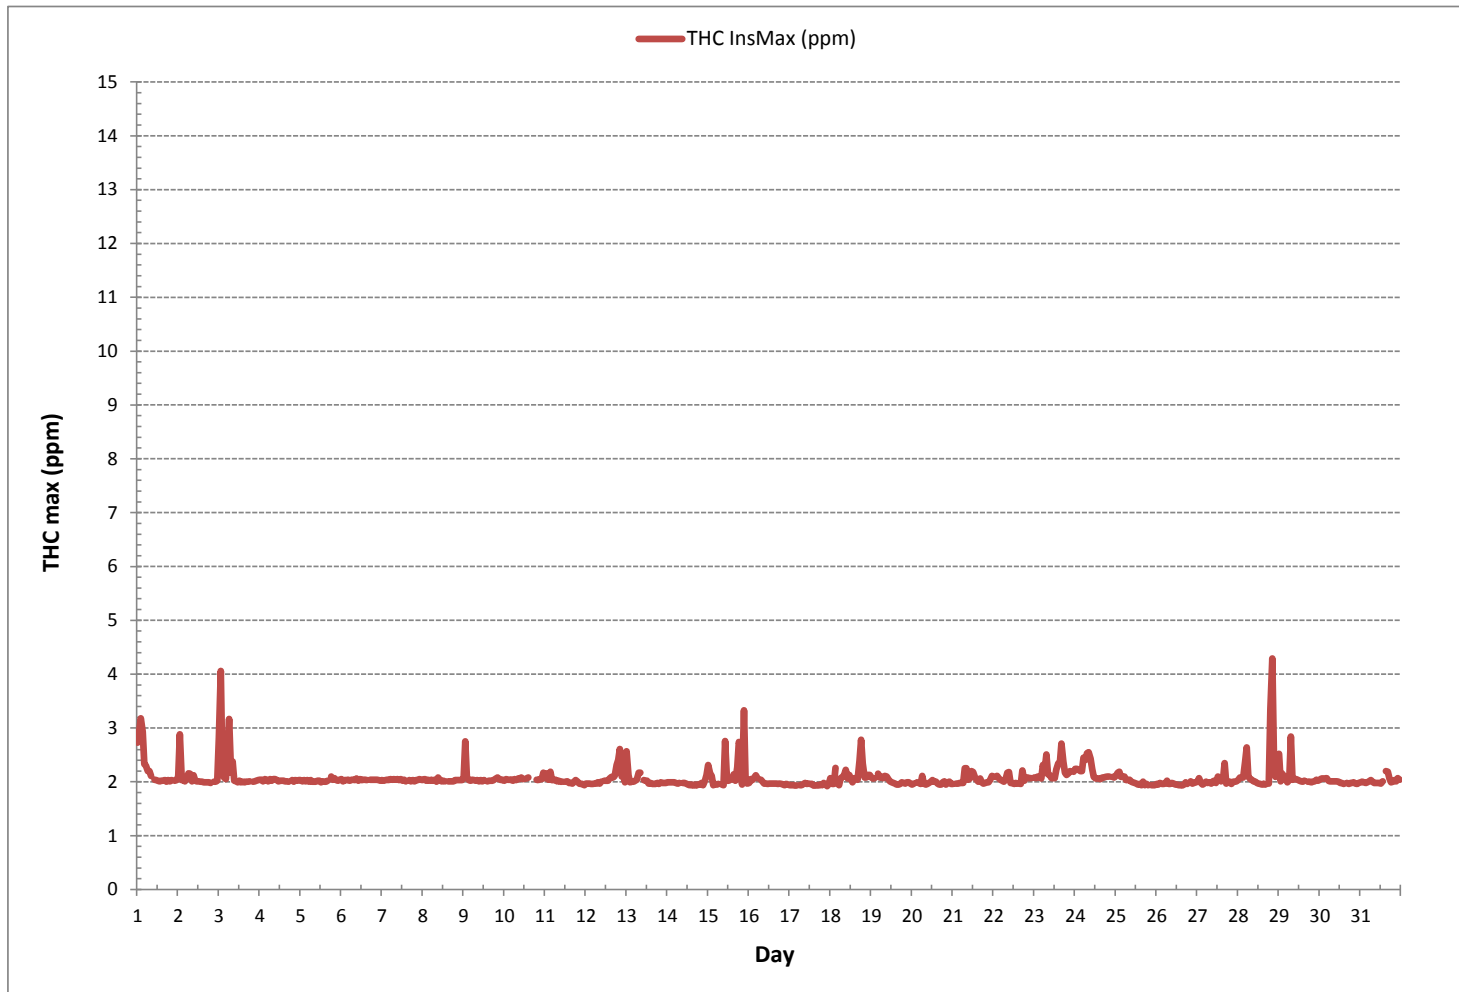



PEACE RIVER AREA MONITORING PROGRAM COMMITTEE  
Three Creeks 986b Station - October 2018

METHANE MAX Instantaneous Maximum (CH<sub>4</sub> ppm)

HR START (MST)	0:00	1:00	2:00	3:00	4:00	5:00	6:00	7:00	8:00	9:00	10:00	11:00	12:00	13:00	14:00	15:00	16:00	17:00	18:00	19:00	20:00	21:00	22:00	23:00	DAILY	DAILY	24-HR	RDGS.
HR END (MST)	0:59	1:59	2:59	3:59	4:59	5:59	6:59	7:59	8:59	9:59	10:59	11:59	12:59	13:59	14:59	15:59	16:59	17:59	18:59	19:59	20:59	21:59	22:59	23:59	MIN.	MAX.	AVG.	
DAY 1	2.73	2.94	3.18	2.93	2.33	2.30	2.20	2.20	2.11	Y	2.04	2.03	2.02	2.01	2.02	2.02	2.03	2.00	2.03	2.01	2.03	S	2.02	2.03	2.00	3.18	2.24	23
2	2.10	2.88	2.03	2.03	2.01	2.07	2.16	2.15	2.01	2.12	2.02	2.01	2.01	2.00	2.00	1.99	1.99	1.99	1.99	1.98	S	2.00	2.00	2.02	1.98	2.88	2.07	24
3	2.82	4.06	2.19	2.08	2.05	2.62	3.17	2.17	2.38	2.02	2.01	1.99	2.02	1.99	2.00	1.99	2.00	2.00	2.01	S	2.00	2.01	2.02	2.03	1.99	4.06	2.24	24
4	2.04	2.04	2.01	2.05	2.04	2.01	2.05	2.02	2.05	2.05	2.03	2.01	2.02	2.02	2.02	2.01	2.01	2.00	S	2.03	2.00	2.03	2.02	2.03	2.00	2.05	2.02	24
5	2.03	2.01	2.03	2.01	2.03	2.00	2.03	2.00	2.00	2.00	2.02	2.02	1.99	2.01	2.00	2.00	2.02	S	2.10	2.04	2.07	2.03	2.02	2.04	1.99	2.10	2.02	24
6	2.05	2.01	2.03	2.03	2.04	2.02	2.04	2.04	2.03	2.06	2.02	2.05	2.03	2.04	2.00	2.03	S	2.04	2.04	2.04	2.04	2.03	2.02	2.02	2.01	2.06	2.03	24
7	2.03	2.02	2.03	2.04	2.03	2.05	2.04	2.05	2.04	2.05	2.03	2.05	2.02	2.04	2.01	S	2.03	2.01	2.03	2.01	2.03	2.03	2.05	2.04	2.01	2.05	2.03	24
8	2.03	2.05	2.02	2.04	2.02	2.04	2.02	2.04	2.00	2.08	2.03	2.01	2.02	2.01	S	2.01	2.01	2.01	2.01	2.03	2.03	2.03	2.03	2.03	2.00	2.08	2.03	24
9	2.08	2.75	2.08	2.03	2.02	2.04	2.03	2.02	2.03	2.01	2.03	2.01	2.03	S	2.01	2.02	2.02	2.02	2.04	2.06	2.08	2.05	2.03	2.04	2.01	2.75	2.07	24
10	2.02	2.05	2.04	2.04	2.04	2.02	2.05	2.03	2.06	2.05	2.08	2.05	S	2.06	2.08	C	C	C	C	2.04	2.03	2.05	2.05	2.17	2.02	2.17	2.05	24
11	2.07	2.16	2.04	2.19	2.03	2.03	2.04	2.01	2.02	2.00	2.00	S	2.00	2.01	1.98	1.98	1.97	2.00	2.03	2.00	1.97	1.96	1.96	1.94	1.94	2.19	2.02	24
12	1.97	1.97	1.97	1.96	1.96	1.97	1.97	1.99	1.97	2.00	S	2.02	2.02	2.02	2.06	2.09	2.08	2.11	2.31	2.41	2.61	2.10	2.21	1.99	1.96	2.61	2.08	24
13	2.57	2.12	1.99	2.00	2.00	2.02	2.04	2.17	2.17	S	2.03	2.02	2.02	1.97	1.98	1.96	1.96	1.96	1.98	1.96	1.99	1.98	1.98	1.98	1.96	2.57	2.04	24
14	1.99	1.99	1.99	1.99	1.99	1.98	1.97	1.98	S	1.98	1.98	1.97	1.95	1.94	1.95	1.93	1.95	1.93	1.95	1.95	1.98	1.94	2.02	2.13	1.93	2.13	1.97	24
15	2.31	2.16	2.11	1.94	1.96	1.95	1.96	S	1.95	1.94	1.96	2.02	2.02	2.04	2.05	2.14	2.02	2.27	2.74	2.74	1.95	3.33	2.00	1.97	1.94	3.33	2.15	24
16	1.98	2.05	2.03	2.08	2.12	2.07	S	2.04	2.00	1.97	1.97	1.96	1.97	1.97	1.97	1.97	1.97	1.96	1.97	1.96	1.95	1.94	1.96	1.95	1.94	2.12	1.99	24
17	1.94	1.94	1.94	1.93	1.93	S	1.94	1.94	1.96	1.98	1.96	1.97	1.96	1.96	1.93	1.93	1.94	1.93	1.95	1.94	1.98	1.95	1.92	1.96	1.92	1.98	1.95	24
18	2.07	1.93	1.94	2.26	S	1.94	2.07	2.09	2.13	2.22	2.06	2.13	2.06	1.99	2.07	2.06	2.04	2.39	2.78	2.34	2.08	2.08	2.13	2.13	1.93	2.78	2.13	24
19	2.08	2.06	2.07	S	2.15	2.08	2.09	2.07	2.11	2.10	2.05	2.01	1.99	1.98	1.97	1.95	1.95	1.96	1.99	1.98	1.97	1.96	1.99	1.97	1.95	2.15	2.02	24
20	1.95	1.97	S	1.99	1.98	1.96	2.11	1.97	1.95	1.96	1.98	2.00	2.03	2.00	2.00	1.97	1.95	1.95	1.99	2.01	1.95	1.99	2.00	1.96	1.95	2.11	1.98	24
21	1.96	S	1.97	1.97	1.98	1.98	1.98	2.25	2.25	2.04	2.06	2.20	2.18	2.08	2.04	2.00	2.06	1.99	1.97	1.98	1.99	1.99	2.03	2.11	1.96	2.25	2.05	24
22	S	2.09	2.11	2.07	2.04	2.02	2.00	2.04	2.17	2.18	1.98	1.98	1.96	1.98	1.97	1.97	1.96	2.21	2.02	2.08	2.08	2.07	2.07	S	1.96	2.21	2.05	24
23	2.08	2.07	2.10	2.10	2.06	2.31	2.18	2.51	2.14	2.13	2.07	2.07	2.07	2.23	2.22	2.34	2.71	2.37	2.17	2.13	2.16	2.20	S	2.19	2.06	2.71	2.20	24
24	2.24	2.24	2.20	2.20	2.18	2.45	2.41	2.46	2.47	2.43	2.24	2.09	2.06	2.05	2.06	2.05	2.08	2.08	2.09	2.10	2.10	S	2.09	2.08	2.05	2.47	2.19	24
25	2.11	2.17	2.16	2.09	2.10	2.10	2.03	2.03	2.04	2.00	1.99	1.98	1.97	1.95	1.96	1.94	2.00	1.94	1.96	1.94	S	1.94	1.94	1.94	1.94	2.17	2.01	24
26	1.96	1.95	1.98	1.96	1.96	1.97	2.02	1.96	1.96	1.98	1.97	1.95	1.95	1.94	1.94	1.93	1.95	1.99	1.96	S	2.01	1.97	1.98	1.99	1.93	2.02	1.97	24
27	2.00	2.07	1.98	1.95	1.97	2.00	1.98	1.99	1.97	2.01	2.02	1.98	2.10	2.04	2.01	2.05	2.35	1.97	S	2.00	1.96	2.00	2.00	2.01	1.95	2.35	2.02	24
28	2.03	2.08	2.08	2.08	2.37	2.64	2.10	2.05	2.04	2.01	2.00	1.98	1.97	1.96	1.95	1.96	1.95	S	1.97	3.35	4.29	2.47	2.09	2.50	1.95	4.29	2.26	24
29	2.52	2.01	2.15	2.10	2.05	1.99	2.03	2.84	2.04	2.05	2.05	2.04	2.02	2.01	2.00	2.02	S	2.00	2.00	1.99	2.00	2.01	2.04	2.02	1.99	2.84	2.09	24
30	2.04	2.06	2.06	2.06	2.07	2.02	2.01	2.01	2.01	2.01	2.01	2.00	1.98	1.98	1.96	S	1.98	1.96	1.98	1.98	1.99	1.97	1.96	1.98	1.96	2.07	2.00	24
31	1.99	2.00	1.99	1.98	1.99	2.01	2.03	2.00	1.98	1.98	1.98	1.98	1.97	2.01	S	2.20	2.19	2.06	1.99	2.00	2.03	2.01	2.07	2.04	1.97	2.20	2.02	24
HOURLY MAX	2.82	4.06	3.18	2.93	2.37	2.64	3.17	2.84	2.47	2.43	2.24	2.20	2.18	2.23	2.22	2.34	2.71	2.39	2.78	3.35	4.29	3.33	2.21	2.50				
HOURLY AVG	2.13	2.20	2.08	2.07	2.05	2.09	2.09	2.10	2.07	2.05	2.02	2.02	2.01	2.01	2.01	2.02	2.04	2.04	2.07	2.11	2.12	2.07	2.02	2.04				


STATUS FLAG CODES

C	- MONTHLY CALIBRATION	Q	- QUALITY ASSURANCE
C1	- REPEAT CALIBRATION	R	- RECOVERY
Y	- MAINTENANCE	X	- MACHINE MALFUNCTION
S	- DAILY ZERO/SPAN CHECK	G	- OUT FOR REPAIR
S1	- REPEAT ZERO/SPAN CHECK	P	- POWER FAILURE

MONTHLY SUMMARY

NUMBER OF NON-ZERO READINGS:	707
MAXIMUM INSTANTANEOUS VALUE:	4.29 ppm @ HOUR 20 ON DAY 28
IZS CALIBRATION TIME:	32 hrs
MONTHLY CALIBRATION TIME:	4 hrs
OPERATIONAL TIME:	743 hrs
STANDARD DEVIATION:	0.20

METHANE MAX Instantaneous Maximum (CH<sub>4</sub> ppm)

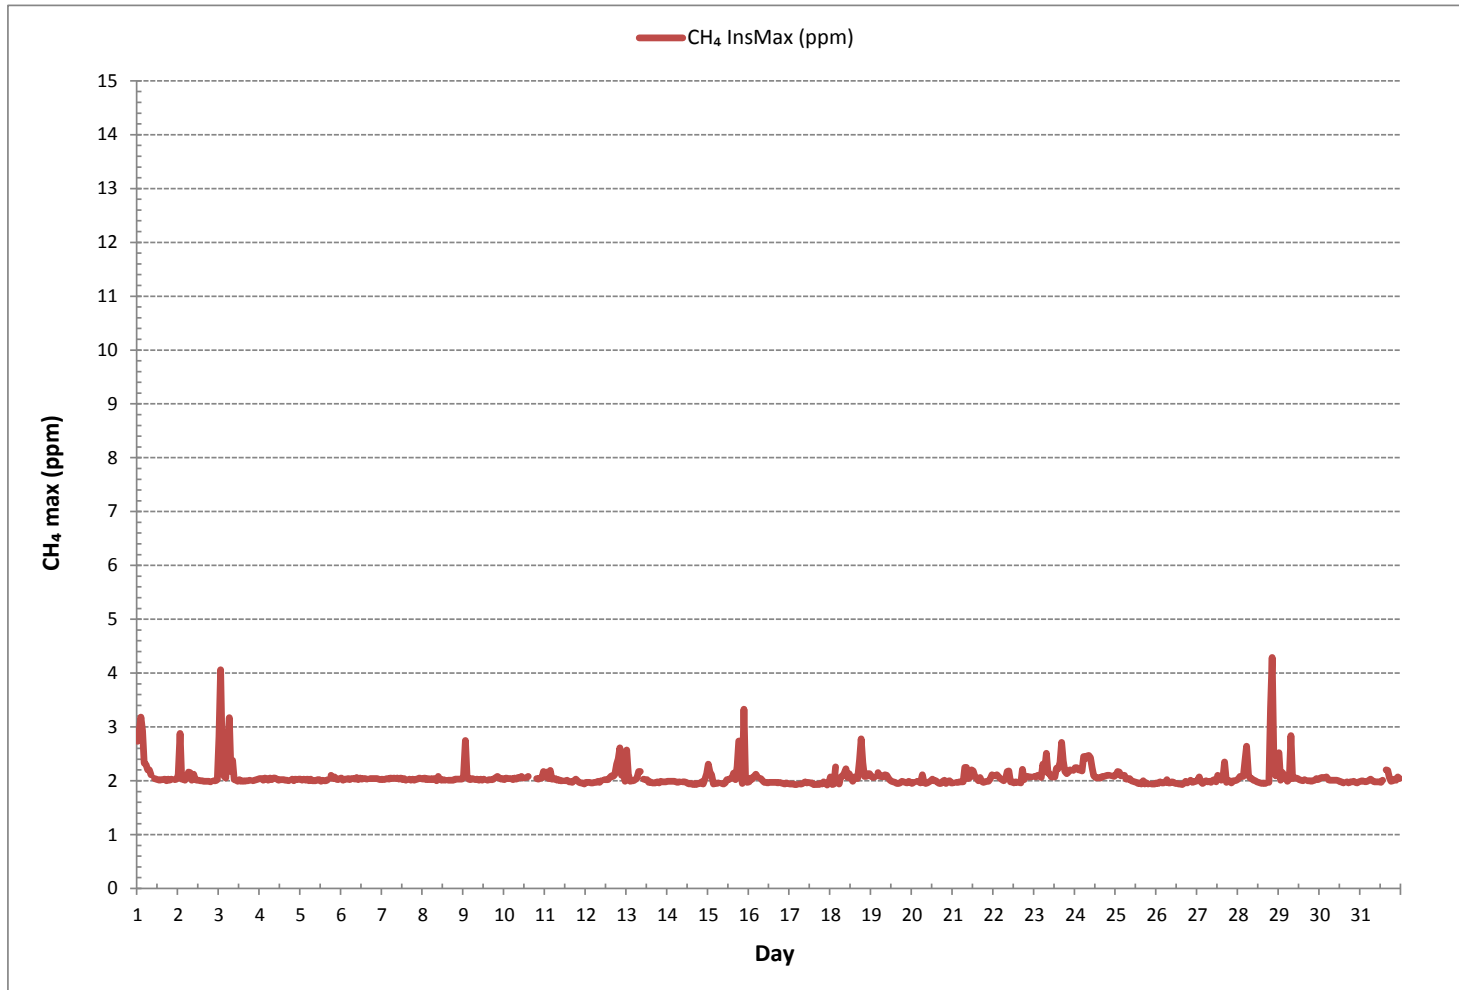





PEACE RIVER AREA MONITORING PROGRAM COMMITTEE  
Three Creeks 986b Station - October 2018

NON-METHANE HYDROCARBONS Instantaneous Maximum (NMHC ppm)

HR START (MST)	0:00	1:00	2:00	3:00	4:00	5:00	6:00	7:00	8:00	9:00	10:00	11:00	12:00	13:00	14:00	15:00	16:00	17:00	18:00	19:00	20:00	21:00	22:00	23:00	DAILY MIN.	DAILY MAX.	24-HR AVG.	RDGS.	
HR END (MST)	0:59	1:59	2:59	3:59	4:59	5:59	6:59	7:59	8:59	9:59	10:59	11:59	12:59	13:59	14:59	15:59	16:59	17:59	18:59	19:59	20:59	21:59	22:59	23:59					
DAY 1	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	Y	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	23	
2	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	24	
3	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	24	
4	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
5	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
6	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
7	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
8	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
9	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
10	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	C	C	C	C	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
11	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
12	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
13	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
14	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
15	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.80	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.80	0.03	24
16	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
17	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
18	0.00	0.04	0.03	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.04	0.00	24	
19	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
20	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
21	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
22	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	24	
23	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.01	0.00	0.04	0.00	0.00	0.00	0.00	0.00	0.05	S	0.00	0.00	0.05	0.00	24
24	0.00	0.00	0.08	0.00	0.07	0.00	0.04	0.09	0.12	0.05	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.12	0.02	24	
25	0.01	0.00	0.12	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.12	0.01	24	
26	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
27	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
28	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
29	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
30	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
31	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	S	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	24	
HOURLY MAX	0.01	0.04	0.12	0.00	0.07	0.00	0.04	0.09	0.12	0.05	0.80	0.00	0.00	0.00	0.01	0.00	0.04	0.00	0.00	0.00	0.00	0.05	0.00	0.00					
HOURLY AVG	0.00	0.00	0.01	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.03	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00	0.00					


STATUS FLAG CODES

C	- MONTHLY CALIBRATION	Q	- QUALITY ASSURANCE
C1	- REPEAT CALIBRATION	R	- RECOVERY
Y	- MAINTENANCE	X	- MACHINE MALFUNCTION
S	- DAILY ZERO/SPAN CHECK	G	- OUT FOR REPAIR
S1	- REPEAT ZERO/SPAN CHECK	P	- POWER FAILURE

MONTHLY SUMMARY

NUMBER OF NON-ZERO READINGS:	14
MAXIMUM INSTANTANEOUS VALUE:	0.80 ppm @ HOUR 10 ON DAY 15
IZS CALIBRATION TIME:	32 hrs
MONTHLY CALIBRATION TIME:	4 hrs
OPERATIONAL TIME:	743 hrs
STANDARD DEVIATION:	0.03

NON-METHANE HYDROCARBONS Instantaneous Maximum (NMHC ppm)

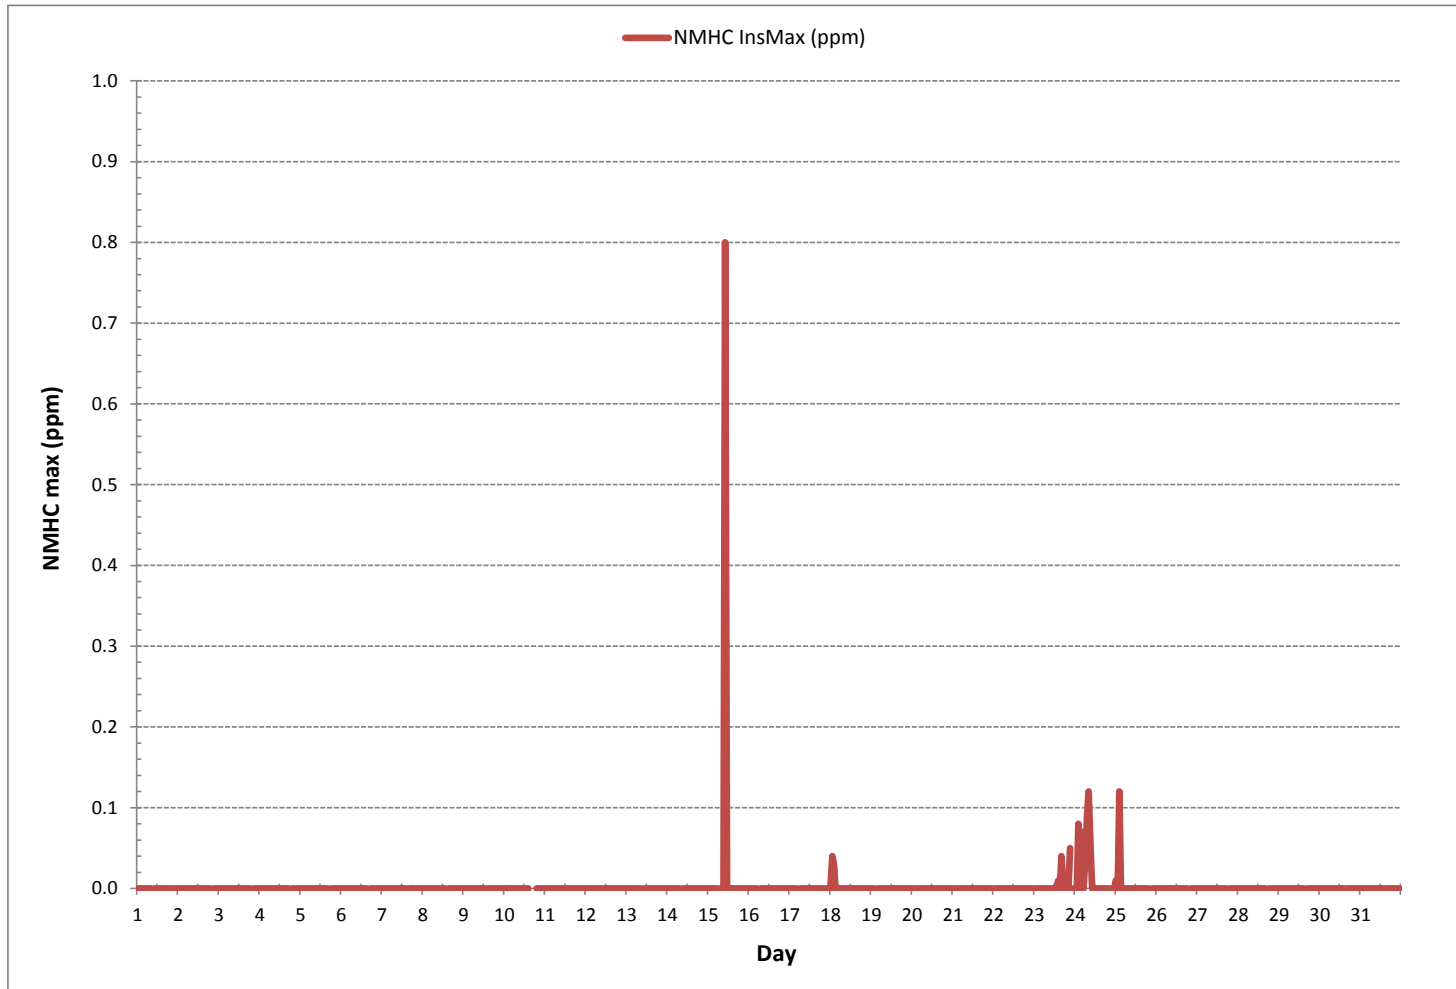



PEACE RIVER AREA MONITORING PROGRAM COMMITTEE  
Three Creeks 986b Station - October 2018

WIND SPEED Instantaneous Maximum (WS kph)

HR START (MST)	0:00	1:00	2:00	3:00	4:00	5:00	6:00	7:00	8:00	9:00	10:00	11:00	12:00	13:00	14:00	15:00	16:00	17:00	18:00	19:00	20:00	21:00	22:00	23:00	DAILY	DAILY	24-HR	RDGS.
HR END (MST)	0:59	1:59	2:59	3:59	4:59	5:59	6:59	7:59	8:59	9:59	10:59	11:59	12:59	13:59	14:59	15:59	16:59	17:59	18:59	19:59	20:59	21:59	22:59	23:59	MIN.	MAX.	AVG.	
DAY 1	5.0	4.5	3.5	4.7	4.9	4.6	3.1	2.8	8.6	16.5	21.6	23.7	24.5	24.7	27.8	31.8	28.2	22.2	27.4	21.9	24.5	19.9	15.6	7.8	2.8	31.8	15.8	24
2	4.7	4.1	5.2	5.1	5.0	4.7	7.3	12.3	13.3	21.3	27.4	27.9	27.4	23.6	26.1	25.6	25.0	21.9	15.3	21.3	21.3	17.3	15.0	8.6	4.1	27.9	16.1	24
3	6.1	4.9	4.3	6.0	4.9	6.0	3.9	3.1	3.1	5.6	14.3	12.1	13.4	12.4	17.9	14.1	8.5	6.1	7.8	10.1	10.8	13.7	12.8	15.2	3.1	17.9	9.0	24
4	13.9	13.4	14.1	13.9	12.7	12.8	10.9	11.7	12.5	15.2	17.0	11.0	13.0	16.9	13.4	19.6	18.3	15.1	10.5	17.0	29.0	13.8	16.4	21.9	10.5	29.0	15.2	24
5	13.5	17.3	18.2	20.2	15.6	18.1	16.6	15.8	16.0	14.0	13.2	15.2	15.2	17.6	14.8	16.6	17.1	13.7	8.5	8.7	21.0	21.3	22.6	20.3	8.5	22.6	16.3	24
6	18.6	17.2	17.4	20.2	14.9	14.4	9.6	16.0	11.0	10.9	11.8	17.3	17.9	22.7	23.1	23.5	23.7	19.8	16.1	15.0	14.0	18.2	18.3	16.6	9.6	23.7	17.0	24
7	20.4	21.8	22.3	26.9	26.3	21.5	22.5	21.6	21.2	21.1	20.3	24.7	24.6	25.8	24.5	25.3	25.2	24.0	21.6	22.0	19.9	20.9	19.6	22.2	19.6	26.9	22.8	24
8	21.2	19.6	22.1	16.9	22.1	19.4	22.4	22.2	26.1	24.3	25.9	25.2	20.9	24.0	21.0	21.9	20.4	19.1	13.6	15.2	16.2	14.3	16.2	15.4	13.6	26.1	20.2	24
9	13.8	3.9	15.4	16.9	13.0	17.1	15.7	15.9	17.6	19.8	21.5	19.5	22.4	19.2	17.9	22.0	21.6	15.7	13.3	12.3	13.1	18.4	20.4	17.1	3.9	22.4	16.8	24
10	16.8	20.9	21.5	17.3	17.5	18.9	17.3	16.8	17.8	9.3	15.4	15.0	15.4	14.2	9.2	8.9	7.2	6.7	5.3	8.7	8.9	7.9	9.8	11.8	5.3	21.5	13.3	24
11	9.8	11.1	7.6	9.4	9.0	17.0	14.2	20.8	23.1	31.5	34.2	28.2	27.5	27.8	26.3	22.8	18.4	14.9	16.7	14.3	11.4	10.0	7.3	8.3	7.3	34.2	17.6	24
12	6.1	3.2	11.6	12.8	16.8	16.6	17.6	16.3	23.6	29.0	26.2	28.4	28.2	24.6	22.3	22.0	16.3	15.5	11.6	8.1	6.4	7.3	5.7	4.1	3.2	29.0	15.8	24
13	4.3	5.0	3.2	2.4	3.4	2.8	3.4	4.4	8.3	10.5	13.5	13.2	13.7	16.0	21.0	17.3	16.4	10.0	10.4	9.3	13.4	16.0	14.6	14.4	2.4	21.0	10.3	24
14	10.1	13.8	11.4	17.9	19.3	18.6	20.9	24.3	23.1	23.2	24.7	24.4	29.7	26.8	31.8	30.7	20.1	24.7	18.0	14.5	20.3	19.4	12.9	16.8	10.1	31.8	20.7	24
15	17.2	21.6	13.4	5.1	9.0	8.9	7.1	7.4	12.0	8.9	7.8	11.5	19.9	19.8	21.5	19.2	15.1	14.7	10.8	5.2	4.1	6.9	4.0	4.3	4.0	21.6	11.5	24
16	4.6	4.9	4.4	5.6	5.8	7.9	6.4	9.5	8.9	9.3	12.5	14.0	17.1	19.4	26.2	26.0	22.5	10.4	14.2	15.5	19.3	21.0	20.4	21.4	4.4	26.2	13.6	24
17	19.4	18.0	15.6	17.2	18.7	20.2	27.8	28.0	31.2	27.8	32.6	30.3	27.9	34.3	33.8	33.1	31.1	17.9	17.1	19.8	35.3	35.3	25.3	25.6	15.6	35.3	26.0	24
18	13.0	12.1	6.5	9.1	8.7	9.3	13.1	25.2	19.0	21.4	15.1	21.1	28.9	36.6	35.6	43.9	38.8	29.1	17.0	15.0	10.2	6.1	4.8	4.8	4.8	43.9	18.5	24
19	4.8	3.4	4.8	6.3	5.7	4.7	4.1	3.6	4.0	5.4	11.5	13.5	15.1	19.2	18.7	23.2	24.2	18.8	14.0	24.5	30.7	17.1	19.3	24.1	3.4	30.7	13.4	24
20	26.8	24.4	24.8	24.4	31.7	23.3	17.9	15.4	29.1	32.2	44.9	49.4	55.8	44.5	54.7	40.7	36.9	32.0	32.3	29.3	32.2	29.4	20.3	22.9	15.4	55.8	32.3	24
21	17.9	14.6	16.2	11.2	7.1	6.5	8.0	9.4	9.4	13.2	22.9	25.3	17.0	19.7	21.6	24.9	16.6	10.8	13.7	11.0	7.8	8.7	9.1	9.2	6.5	25.3	13.8	24
22	9.5	8.6	10.6	13.3	11.9	15.7	11.9	9.4	16.2	19.0	29.2	22.4	22.6	20.3	18.0	15.4	13.9	6.6	4.9	5.1	7.0	12.2	13.6	12.5	4.9	29.2	13.7	24
23	9.0	11.2	8.7	9.4	10.8	6.5	5.2	6.3	6.3	15.3	16.1	10.0	9.4	11.3	9.2	6.6	7.2	3.4	3.5	5.2	4.9	4.1	5.1	8.7	3.4	16.1	8.1	24
24	7.9	5.6	5.3	11.3	7.9	6.1	6.5	7.4	6.4	6.1	10.9	12.4	11.8	14.9	15.5	12.1	14.7	10.2	11.1	6.7	5.7	8.8	6.8	7.2	5.3	15.5	9.1	24
25	6.1	5.6	6.5	8.6	8.9	7.3	10.6	10.8	11.0	20.2	13.1	13.8	15.9	19.7	23.0	21.3	17.3	14.7	25.6	28.4	37.8	23.5	19.5	26.2	5.6	37.8	16.5	24
26	21.6	21.8	15.5	12.9	11.7	12.3	40.5	19.5	8.7	8.9	16.8	18.2	12.9	17.1	26.9	16.4	9.2	8.6	19.0	18.6	10.7	14.9	20.7	22.4	8.6	40.5	16.9	24
27	25.1	14.1	21.5	25.5	29.6	35.4	27.0	24.7	25.2	23.2	25.8	29.7	26.1	35.9	48.0	31.3	10.8	6.2	6.0	4.7	4.7	4.6	4.4	5.9	4.4	48.0	20.6	24
28	9.3	8.6	9.7	9.5	8.3	8.2	7.0	8.5	11.1	11.4	11.5	15.2	12.9	14.9	14.2	17.7	12.5	8.9	7.1	4.0	3.3	7.2	9.9	11.5	3.3	17.7	10.1	24
29	7.8	7.5	6.6	9.7	7.6	5.6	6.3	7.0	9.6	11.6	13.7	11.9	14.0	14.9	17.6	14.9	11.7	7.3	7.4	9.2	7.2	6.2	6.4	6.1	5.6	17.6	9.5	24
30	6.7	5.8	6.2	7.3	5.8	5.4	5.2	4.1	5.5	10.1	13.0	13.4	12.0	12.0	18.8	19.5	13.8	8.3	8.3	8.5	7.2	10.9	15.5	13.4	4.1	19.5	9.9	24
31	11.9	12.8	8.0	6.8	8.3	8.7	8.7	6.4	6.9	12.1	14.2	15.2	17.9	14.2	10.1	5.2	11.2	15.8	17.7	22.2	24.2	24.0	24.1	24.8	5.2	24.8	13.8	24
HOURLY MAX	26.8	24.4	24.8	26.9	31.7	35.4	40.5	28.0	31.2	32.2	44.9	49.4	55.8	44.5	54.7	43.9	38.8	32.0	32.3	29.3	37.8	35.3	25.3	26.2				


STATUS FLAG CODES

C	- MONTHLY CALIBRATION	Q	- QUALITY ASSURANCE
C1	- REPEAT CALIBRATION	R	- RECOVERY
Y	- MAINTENANCE	X	- MACHINE MALFUNCTION
S	- DAILY ZERO/SPAN CHECK	G	- OUT FOR REPAIR
S1	- REPEAT ZERO/SPAN CHECK	P	- POWER FAILURE

MONTHLY SUMMARY

MAXIMUM INSTANTANEOUS VALUE:	55.8	kph	@ HOUR	12	ON DAY	20	
OPERATIONAL TIME:						744	hrs

WIND SPEED Instantaneous Maximum (WS kph)

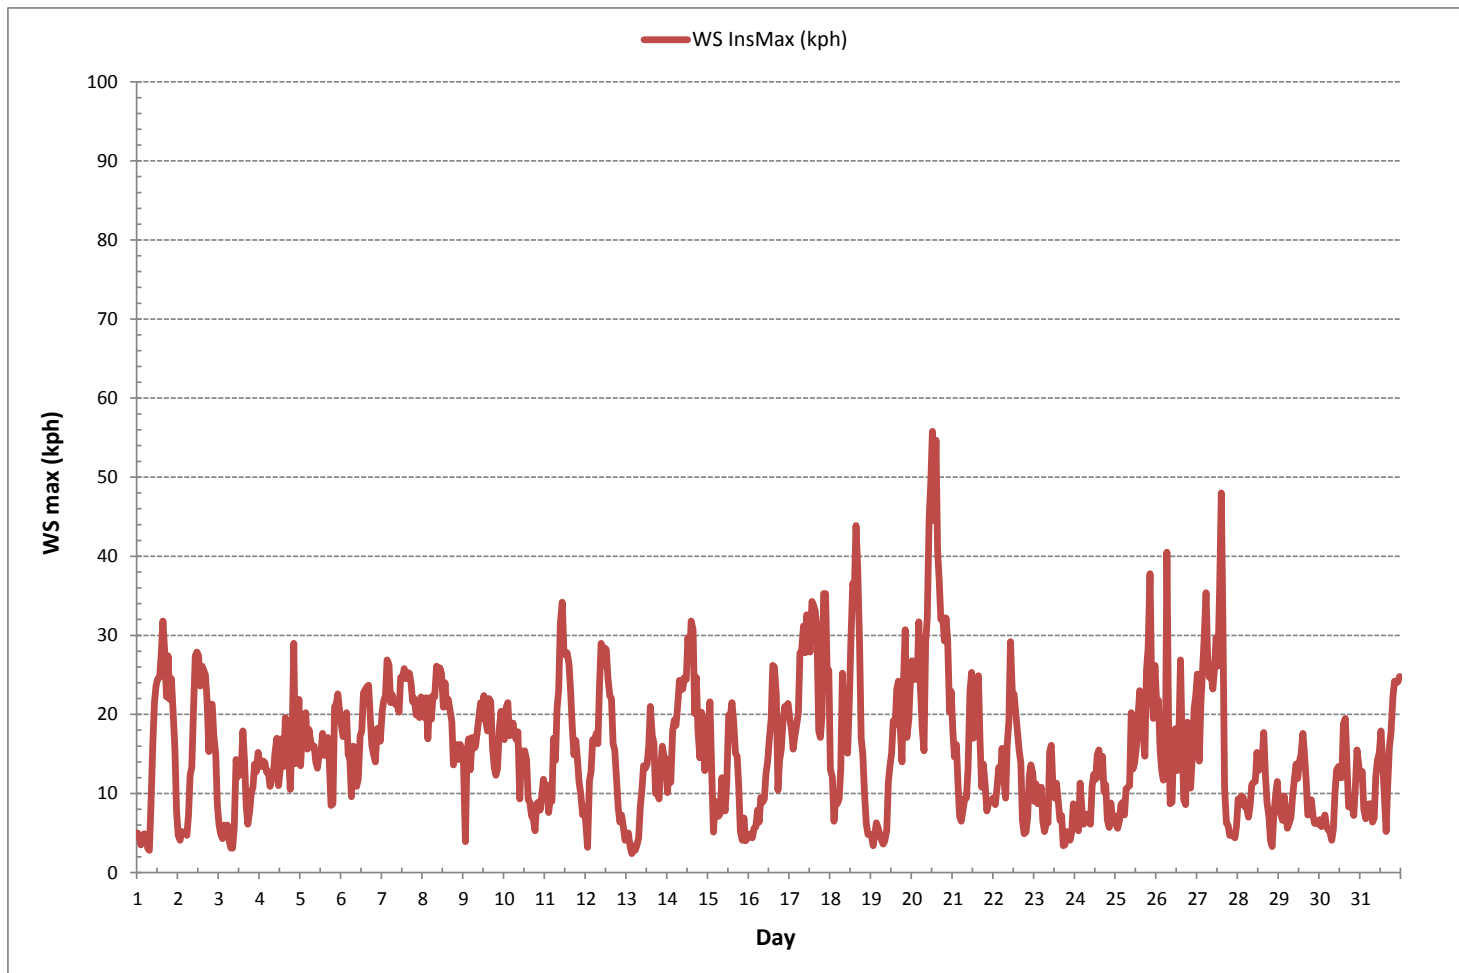


***APPENDIX IV***  
***REPORT CERTIFICATION FORM***

### Report Certification Form

Alberta Airshed (if applicable)	EPA Approval or Code of Practice Registration # (if applicable)
YES	NA
Company Name (if applicable)	Industrial Operation Name (if applicable)
Peace River Area Monitoring Program Committee	Three Creeks 986b Station
Name of the Representative of the Person Responsible	Position / Title of the Representative of the Person Responsible
Mike Bisaga / Lily Lin	Technical Program Managers
Is an External Party Certifying the Report? (If 'Yes', fill in the fields below for the external person.)	
<input checked="" type="checkbox"/> Yes <input type="checkbox"/> No	
Name of External Person Certifying the Report	Position / Title of External Person Certifying the Report
Cheri Sinclair	Supervisor, Customer Service, Air Services
Company Name for the External Person Certifying the Report	Identification of Qualifications / Professional Designations of the External Person Certifying the Report
Maxxam Analytics, A Bureau Veritas Group Company	B.Sc.

Maxxam Analytics is the designated contractor conducting monitoring and reporting activities. I certify that the submitted data has been (a) reviewed and validated as per the AMD Chapter 6: Ambient Data Quality. I certify that the submitted report (b) accurately reflects the monitoring results and reporting timeframe and (c) meets the specified analysis, summarization and reporting requirements as per the AMD Chapter 9: Reporting.



Signature of the External Person Certifying the Report

19 - Nov - 2018





Report Issued Date (dd-mon-yyyy)

***APPENDIX V***  
***DATA VALIDATION CERTIFICATION FORM***



### Validation Certificate Form

<b>Client:</b> <u>Peace River Area Monitoring Program Committee</u>	<b>Project #:</b> <u>8449-2018-10-67-C</u>
<b>Site:</b> <u>Three Creeks 986b Station</u>	<b>Contact:</b> <u>Karla Reesor</u>

Level 0 Preliminary Verification	<u></u>	Date <u>15 - Nov - 2018</u>
Level 1 Primary Validation	<u></u>	Date <u>15 - Nov - 2018</u>
Level 2 Final Validation	<u></u>	Date <u>16 - Nov - 2018</u>
Level 3 Independent Data Review	<u></u>	Date <u>19 - Nov - 2018</u>
Post-Final Validation	<u>NA</u>	Date <u>NA</u>

<b>Notes</b>
The Post-Final Validation step serves to re-evaluate the data that errors or omissions are discovered and/or suspected after the initial submittal of data. This validation is performed on an annual basis.